

Calibration Report

Job Ref.: Data Logger Test

Thermocouple: Calibration Set 1

Test Person Kevin Taylor

Sign: VALID ESIG

Date: 30/03/2011 dd/mm/yyyy Time: 09:57:24

Reviewed By:

Sign:

Date: 30/03/2011 dd/mm/yyyy Time: 10:40:24

EQUIPMENT Logger / Recorder

| | |
|--------------|-----------|
| Manufacturer | Fluke |
| Model | Netdaq |
| Serial No. | 67382 |
| Test House | N/A |
| Cert. No. | 1035 |
| Renew Date | 15/8/2011 |

STABILITY SET-UP

0.15 Degrees per minute for 5 minutes.

Allowed deviation from Reference 2 degrees.

Reference stability criteria 0.05 degrees for 1 minute.

Report after Calibration for 2 minutes every 15 seconds.

Report max deviation allowed 0.2 degrees.

| Setpoints | | Programmed | Reference |
|-----------|-----------|------------|-----------|
| | Low | 50 °C | 50.01 °C |
| | High | 138 °C | 137.99 °C |
| | 1st Check | 121 °C | 121.01 °C |

LOW Point 50.01 °C STABILITY REPORT

Start Time: 09:58:04 Time when stability requirements met: 10:03:06

Elapsed time: 00:05:02

Reference change: 0.03 °C

Maximum sensor change over last minute: 0.1 °C

| | Chan1 | Chan2 | Chan3 |
|-------------|-------|-------|-------|
| Change (°C) | 0.0 | 0.0 | 0.1 |

LOW Point 50.01 °C QUALIFICATION REPORT

| Time | Ref. (°C) | Chan1 | Chan2 | Chan3 |
|----------------|-----------|-------|-------|-------|
| 10:03:06 | 50.01 | 49.9 | 50.1 | 50.0 |
| Deviation (°C) | | - 0.1 | 0.1 | 0.0 |

LOW Point 50.01 °C POST CALIBRATION REPORT

| Time | Ref. | Chan1 | Chan2 | Chan3 |
|----------------|----------|-------|-------|-------|
| 10:03:22 | 50.01 °C | 50.0 | 50.0 | 50.1 |
| Deviation (°C) | | 0.0 | 0.0 | 0.1 |
| 10:03:37 | 49.97 °C | 50.0 | 50.0 | 50.0 |
| Deviation (°C) | | 0.0 | 0.0 | 0.0 |
| 10:03:52 | 50.01 °C | 50.0 | 50.0 | 50.1 |
| Deviation (°C) | | 0.0 | 0.0 | 0.1 |
| 10:04:07 | 50.02 °C | 50.0 | 50.0 | 50.1 |
| Deviation (°C) | | 0.0 | 0.0 | 0.1 |
| 10:04:22 | 50.00 °C | 50.0 | 50.0 | 50.1 |
| Deviation (°C) | | 0.0 | 0.0 | 0.1 |
| 10:04:37 | 50.01 °C | 50.0 | 50.0 | 50.1 |
| Deviation (°C) | | 0.0 | 0.0 | 0.1 |
| 10:04:52 | 49.99 °C | 50.0 | 50.0 | 50.1 |
| Deviation (°C) | | 0.0 | 0.0 | 0.1 |
| MAX DEV. (°C) | | 0.0 | 0.0 | 0.1 |

HIGH Point 137.99 °C STABILITY REPORT

Start Time: 10:05:12 Time when stability requirements met: 10:24:51

Elapsed time: 00:19:40

Reference change: 0.04 °C

Maximum sensor change over last minute: 0.1 °C

| | Chan1 | Chan2 | Chan3 |
|-------------|-------|-------|-------|
| Change (°C) | 0.1 | 0.0 | 0.1 |

HIGH Point 137.99 °C QUALIFICATION REPORT

| Time | Ref. (°C) | Chan1 | Chan2 | Chan3 |
|----------------|-----------|-------|-------|-------|
| 10:24:51 | 137.99 | 137.7 | 138.2 | 138.0 |
| Deviation (°C) | | - 0.3 | 0.2 | 0.0 |

Calibration Report

Job Ref.: Data Logger Test

Thermocouple: Calibration Set 1

Test Person Kevin Taylor

Sign: VALID ESIG

Date: 30/03/2011 dd/mm/yyyy Time: 09:57:24

Reviewed By:

Sign:

Date: 30/03/2011 dd/mm/yyyy Time: 10:40:24

Date:

HIGH Point 137.99 °C POST CALIBRATION REPORT

| Time | Ref. | Chan1 | Chan2 | Chan3 |
|----------------|-----------|-------|-------|-------|
| 10:25:07 | 138.01 °C | 138.0 | 138.0 | 138.0 |
| Deviation (°C) | | 0.0 | 0.0 | 0.0 |
| 10:25:22 | 138.00 °C | 138.0 | 138.0 | 138.0 |
| Deviation (°C) | | 0.0 | 0.0 | 0.0 |
| 10:25:37 | 137.97 °C | 138.0 | 138.0 | 138.0 |
| Deviation (°C) | | 0.0 | 0.0 | 0.0 |
| 10:25:52 | 137.99 °C | 138.0 | 138.0 | 138.0 |
| Deviation (°C) | | 0.0 | 0.0 | 0.0 |
| 10:26:07 | 138.00 °C | 138.1 | 138.0 | 138.0 |
| Deviation (°C) | | 0.1 | 0.0 | 0.0 |
| 10:26:22 | 138.03 °C | 138.0 | 138.0 | 138.0 |
| Deviation (°C) | | 0.0 | 0.0 | 0.0 |
| 10:26:37 | 138.02 °C | 138.0 | 138.0 | 138.0 |
| Deviation (°C) | | 0.0 | 0.0 | 0.0 |
| MAX DEV. (°C) | | 0.1 | 0.0 | 0.0 |

CALIBRATION FACTOR AND OFFSET RESULTS

| Channel Number | Status | High Ref. | High Measured | Low Ref. | Low Measured |
|----------------|----------|-----------|---------------|----------|--------------|
| 1 | IN SPEC. | 137.99 °C | 137.7 °C | 50.01 °C | 49.9 °C |
| 2 | IN SPEC. | 137.99 °C | 138.2 °C | 50.01 °C | 50.1 °C |
| 3 | IN SPEC. | 137.99 °C | 138.0 °C | 50.01 °C | 50.0 °C |

FIRST CALIBRATION CHECK Point 121.01 °C STABILITY REPORT AFTER ADJUSTMENT

Start Time: 10:26:55

Time when stability requirements met: 10:35:06

Elapsed time: 00:08:11

Reference change: 0.04 °C

Maximum sensor change over last minute: 0.1 °C

| Change (°C) | Chan1 | Chan2 | Chan3 |
|-------------|-------|-------|-------|
| | 0.1 | 0.1 | 0.1 |


FIRST CALIBRATION CHECK Point 121.01 °C QUALIFICATION REPORT

| Time | Ref. (°C) | Chan1 | Chan2 | Chan3 |
|----------------|-----------|-------|-------|-------|
| 10:35:06 | 121.01 | 121.0 | 121.0 | 121.1 |
| Deviation (°C) | | 0.0 | 0.0 | 0.1 |

FIRST CALIBRATION CHECK Point 121.01 °C REPORT

| Time | Ref. | Chan1 | Chan2 | Chan3 |
|----------------|-----------|-------|-------|-------|
| 10:35:22 | 121.01 °C | 121.0 | 120.9 | 121.0 |
| Deviation (°C) | | 0.0 | -0.1 | 0.0 |
| 10:35:37 | 120.93 °C | 121.0 | 121.0 | 121.1 |
| Deviation (°C) | | 0.1 | 0.1 | 0.2 |
| 10:35:52 | 120.99 °C | 121.1 | 121.0 | 121.1 |
| Deviation (°C) | | 0.1 | 0.0 | 0.1 |
| 10:36:07 | 121.01 °C | 121.1 | 121.0 | 121.1 |
| Deviation (°C) | | 0.1 | 0.0 | 0.1 |
| 10:36:22 | 121.02 °C | 121.0 | 121.0 | 121.1 |
| Deviation (°C) | | 0.0 | 0.0 | 0.1 |
| 10:36:37 | 120.99 °C | 121.0 | 121.0 | 121.0 |
| Deviation (°C) | | 0.0 | 0.0 | 0.0 |
| 10:36:52 | 121.02 °C | 121.0 | 121.0 | 121.1 |
| Deviation (°C) | | 0.0 | 0.0 | 0.1 |
| MAX DEV. (°C) | | 0.1 | -0.1 | 0.2 |

Data Logger Test
 Cycle No. 000006
 Serial No. Z0278
LTE Scientific Limited
 C:\logsys\Z0278\data\000006.mbf
 01/04/2011
 Lab Fluid 134C : 5 3 Probes

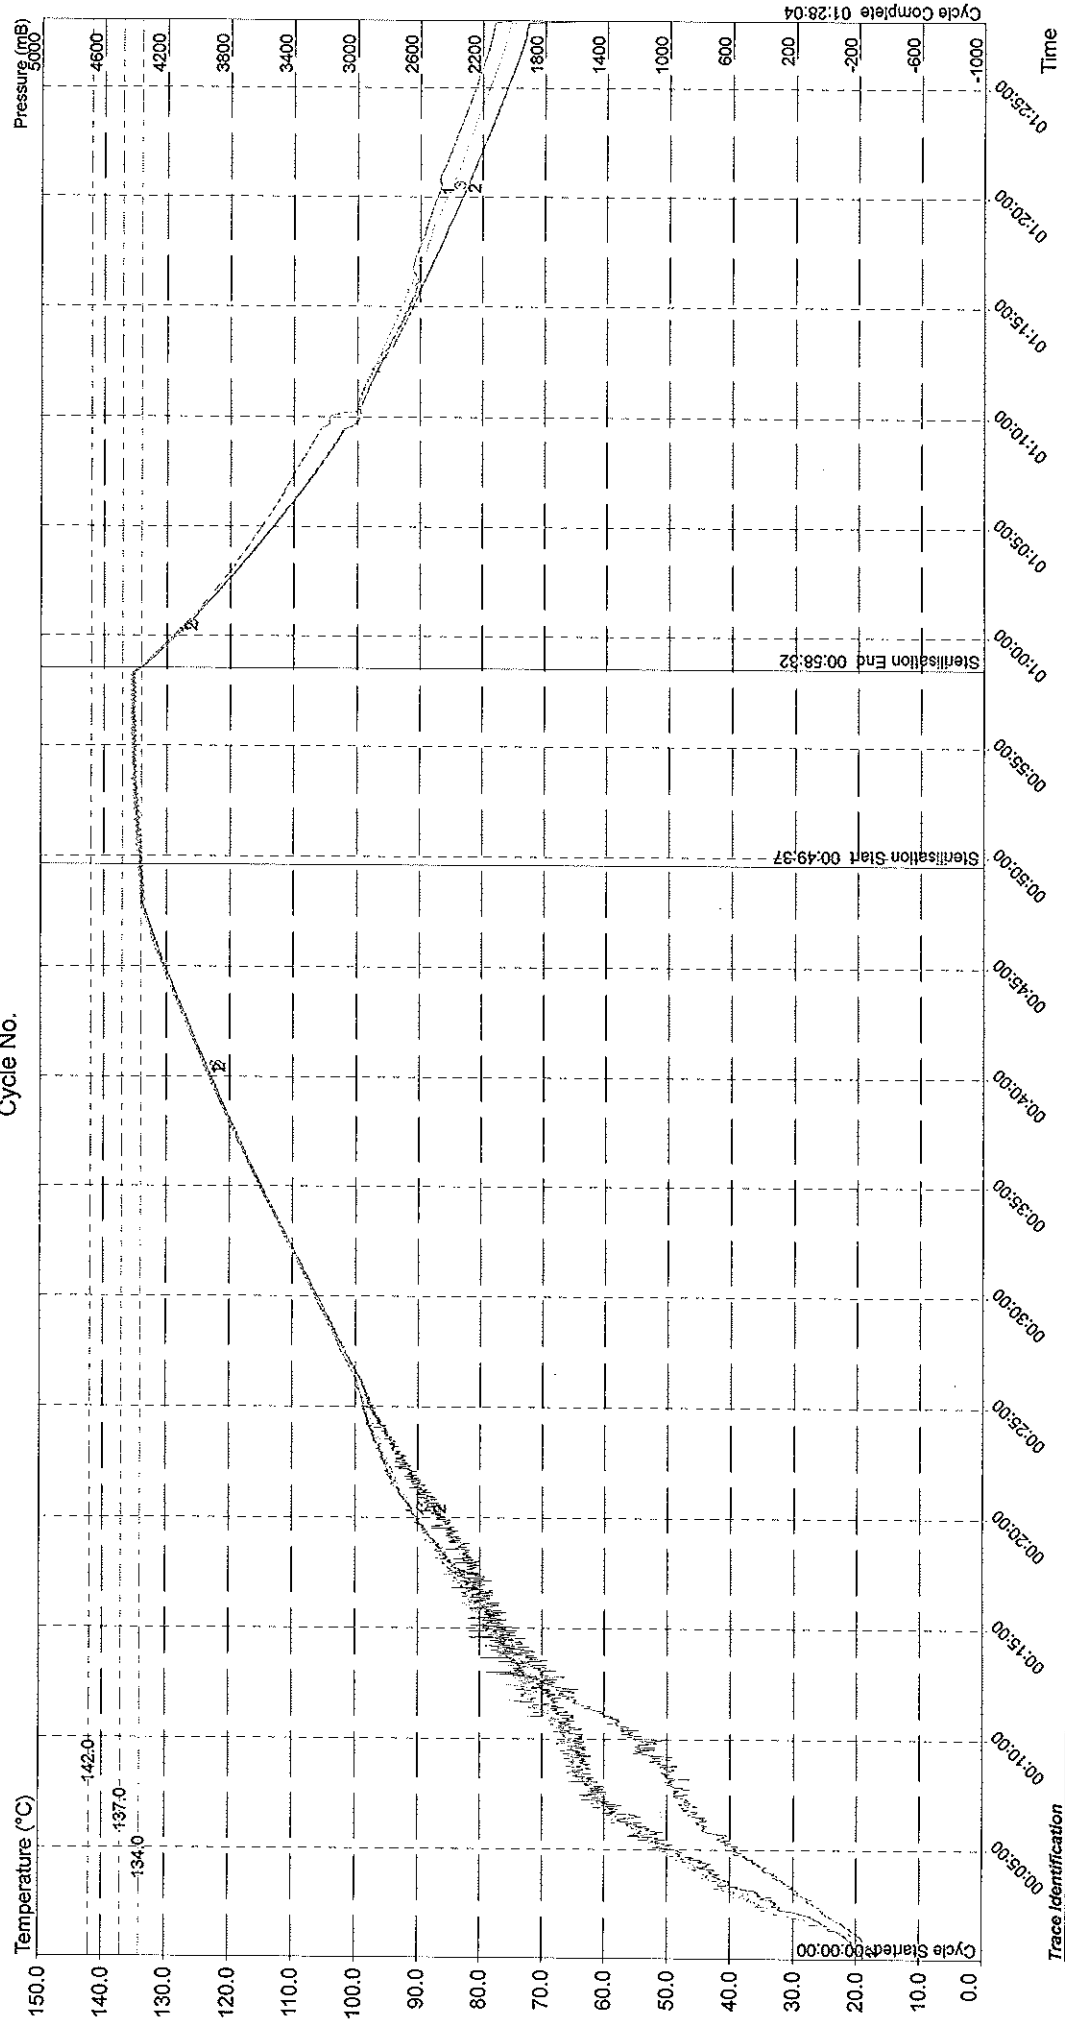


Trace Identification
 1 Drain
 2 Load Probe / Logger
 3 FreeSpace
 13 Press

LTE Scientific Limited

Data Logger Test
 Cycle No. 000006
 Serial No. Z0278

C:\logsys\Z0278\data\0000006.mbf
 01/04/2011
 Lab Fluid 134C : 5 3 Probes

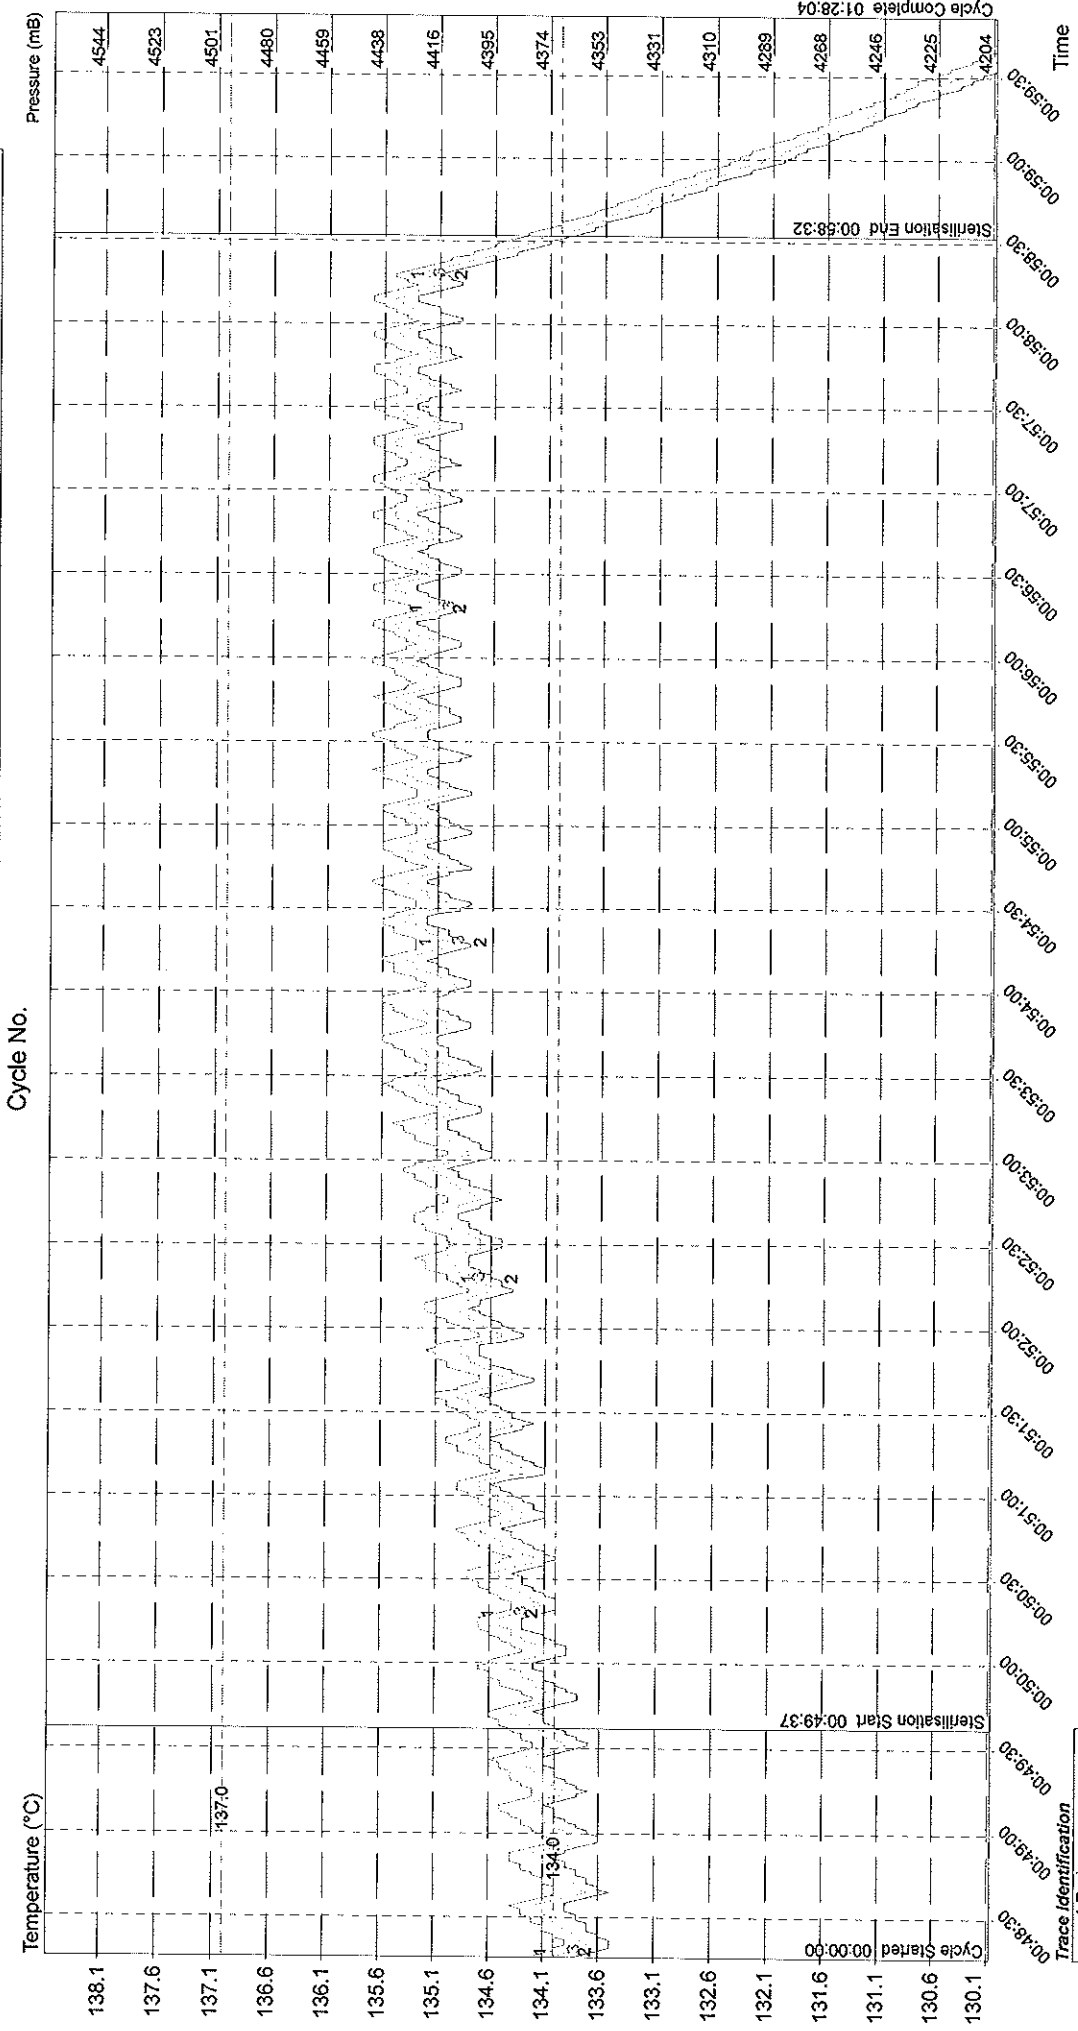

Data Logger Test

LTE Scientific Limited

Cycle No. 000006

01/04/2011

Serial No. Z0278

Lab Fluid 134C : 5 3 Probes

C:\logsys\Z0278\data\000006.mbf

Test Person Kevin Taylor

Sign VALID ESIG

Date 01/04/2011 dd/mm/yyyy 11:30:09

Reviewed By:

Sign

Date dd/mm/yyyy


| Time | Tmp 1 °C | Tmp 2 °C | Tmp 3 °C | Press mB |
|----------|---------------------|-------------|-------------|-------------|
| 00:00:00 | Cycle Started | | | |
| 00:00:04 | 18.7 | 19.0 | 18.9 | -1010 |
| 00:00:05 | 18.7 | 19.0 | 18.9 | -1010 |
| 00:02:05 | 25.1 | 28.8 | 32.9 | -1011 |
| 00:04:05 | 34.6 | 42.5 | 44.9 | -1011 |
| 00:06:05 | 43.7 | 54.8 | 56.0 | -1010 |
| 00:08:05 | 49.4 | 65.0 | 65.6 | -1011 |
| 00:10:05 | 55.5 | 63.8 | 65.6 | -1010 |
| 00:12:05 | 67.4 | 68.3 | 73.0 | -1009 |
| 00:14:05 | 74.4 | 75.8 | 75.8 | -1011 |
| 00:16:05 | 79.2 | 77.2 | 80.6 | -1011 |
| 00:18:05 | 85.1 | 82.5 | 85.8 | -1012 |
| 00:20:05 | 90.2 | 86.8 | 90.1 | -1011 |
| 00:22:05 | 94.6 | 90.1 | 94.3 | -1012 |
| 00:24:05 | 97.6 | 96.8 | 97.1 | -1010 |
| 00:26:05 | 99.7 | 98.9 | 99.3 | -1012 |
| 00:28:05 | 103.2 | 102.7 | 103.0 | -1010 |
| 00:30:05 | 106.6 | 106.3 | 106.5 | -1011 |
| 00:32:05 | 110.2 | 109.8 | 110.0 | -1011 |
| 00:34:05 | 113.6 | 113.3 | 113.5 | -1010 |
| 00:36:05 | 117.1 | 116.7 | 116.9 | -1010 |
| 00:38:05 | 120.4 | 120.0 | 120.2 | -1012 |
| 00:40:05 | 123.5 | 123.0 | 123.2 | -1012 |
| 00:42:05 | 126.5 | 126.1 | 126.3 | -1012 |
| 00:44:05 | 129.4 | 128.9 | 129.1 | -1012 |
| 00:46:05 | 132.0 | 131.5 | 131.7 | -1012 |
| 00:48:05 | 134.0 | 133.6 | 133.7 | -1011 |
| 00:48:51 | 134.4 | 134.0 | 134.1 | -1011 |
| 00:48:56 | 134.1 | 133.7 | 133.8 | -1011 |
| 00:49:15 | 134.2 | 133.7 | 133.9 | -1012 |
| 00:49:20 | 134.4 | 134.0 | 134.1 | -1012 |
| 00:49:31 | 134.2 | 133.7 | 133.9 | -1012 |
| 00:49:37 | Sterilisation Start | | | |
| 00:49:37 | 134.4 | 134.0 | 134.2 | -1011 |
| 00:50:05 | 134.3 | 133.9 | 134.1 | -1012 |
| 00:52:05 | 135.1 | 134.7 | 134.8 | -1011 |
| 00:54:05 | 135.3 | 134.9 | 135.1 | -1012 |
| 00:56:05 | 135.3 | 134.9 | 135.1 | -1012 |
| 00:58:05 | 135.5 | 135.1 | 135.3 | -1012 |
| 00:58:32 | Sterilisation End | | | |
| 00:58:34 | 134.2 | 133.7 | 133.9 | -1012 |
| 01:00:05 | 128.6 | 128.2 | 128.4 | -1011 |
| 01:02:05 | 122.4 | 121.7 | 121.9 | -1012 |
| 01:04:05 | 117.2 | 115.7 | 115.9 | -1012 |
| 01:06:05 | 112.5 | 110.2 | 110.4 | -1009 |

| Time | Tmp 1 | Tmp 2 | Tmp 3 | Press |
|----------|----------------|-------|-------|-------|
| | °C | °C | °C | mB |
| 01:08:05 | 108.5 | 105.1 | 105.4 | -1011 |
| 01:10:05 | 103.8 | 99.6 | 99.9 | -1010 |
| 01:12:05 | 97.2 | 96.8 | 97.6 | -1010 |
| 01:14:05 | 93.3 | 92.7 | 94.2 | -1011 |
| 01:16:05 | 90.4 | 89.4 | 91.3 | -1012 |
| 01:18:05 | 89.5 | 86.1 | 88.3 | -1010 |
| 01:20:05 | 87.1 | 83.0 | 85.5 | -1010 |
| 01:22:05 | 84.9 | 80.1 | 82.7 | -1009 |
| 01:24:05 | 82.3 | 77.3 | 80.1 | -1012 |
| 01:26:05 | 79.9 | 74.6 | 77.5 | -1012 |
| 01:28:04 | Cycle Complete | | | |
| 01:28:04 | 75.2 | 61.1 | 66.1 | -1011 |


| | | CH1 | |
|----|------------|----------|--------|
| 1 | 01/04/2011 | 10:01:01 | 21.93 |
| 2 | 01/04/2011 | 10:03:01 | 25.71 |
| 3 | 01/04/2011 | 10:05:01 | 41.49 |
| 4 | 01/04/2011 | 10:07:01 | 56.47 |
| 5 | 01/04/2011 | 10:09:01 | 65.08 |
| 6 | 01/04/2011 | 10:11:01 | 69.41 |
| 7 | 01/04/2011 | 10:13:01 | 71.88 |
| 8 | 01/04/2011 | 10:15:01 | 76.65 |
| 9 | 01/04/2011 | 10:17:01 | 80.06 |
| 10 | 01/04/2011 | 10:19:01 | 81.85 |
| 11 | 01/04/2011 | 10:21:01 | 86.25 |
| 12 | 01/04/2011 | 10:23:01 | 91.51 |
| 13 | 01/04/2011 | 10:25:01 | 95.78 |
| 14 | 01/04/2011 | 10:27:01 | 98.81 |
| 15 | 01/04/2011 | 10:29:01 | 102.28 |
| 16 | 01/04/2011 | 10:31:01 | 105.81 |
| 17 | 01/04/2011 | 10:33:01 | 109.4 |
| 18 | 01/04/2011 | 10:35:01 | 112.86 |
| 19 | 01/04/2011 | 10:37:01 | 116.27 |
| 20 | 01/04/2011 | 10:39:01 | 119.55 |
| 21 | 01/04/2011 | 10:41:01 | 122.71 |
| 22 | 01/04/2011 | 10:43:01 | 125.61 |
| 23 | 01/04/2011 | 10:45:01 | 128.4 |
| 24 | 01/04/2011 | 10:47:01 | 131.06 |
| 25 | 01/04/2011 | 10:49:01 | 133.29 |
| 26 | 01/04/2011 | 10:51:01 | 133.78 |
| 27 | 01/04/2011 | 10:53:01 | 134.28 |
| 28 | 01/04/2011 | 10:55:01 | 134.71 |
| 29 | 01/04/2011 | 10:57:01 | 134.84 |
| 30 | 01/04/2011 | 10:59:01 | 134.9 |
| 31 | 01/04/2011 | 11:01:01 | 128.77 |
| 32 | 01/04/2011 | 11:03:01 | 122.52 |
| 33 | 01/04/2011 | 11:05:01 | 116.58 |
| 34 | 01/04/2011 | 11:07:01 | 111.01 |
| 35 | 01/04/2011 | 11:09:01 | 105.81 |
| 36 | 01/04/2011 | 11:11:01 | 100.3 |
| 37 | 01/04/2011 | 11:13:01 | 97.08 |
| 38 | 01/04/2011 | 11:15:01 | 92.93 |
| 39 | 01/04/2011 | 11:17:01 | 89.53 |
| 40 | 01/04/2011 | 11:19:01 | 86.37 |
| 41 | 01/04/2011 | 11:21:01 | 83.15 |
| 42 | 01/04/2011 | 11:23:01 | 80.18 |
| 43 | 01/04/2011 | 11:25:01 | 77.33 |
| 44 | 01/04/2011 | 11:27:01 | 74.61 |
| 45 | 01/04/2011 | 11:29:01 | 69.1 |

SL55T, Serial Number: 3400000015699F41

| | |
|---------------------|--------------|
| Time/Date | CH1 |
| 01/04/2011 10:03:01 | 25.707 |
| 01/04/2011 11:29:01 | 69.099 |
| 1 Hours 26 Mins | 43.391 |
| Time >= 134.0°C | 8m 0s [PASS] |

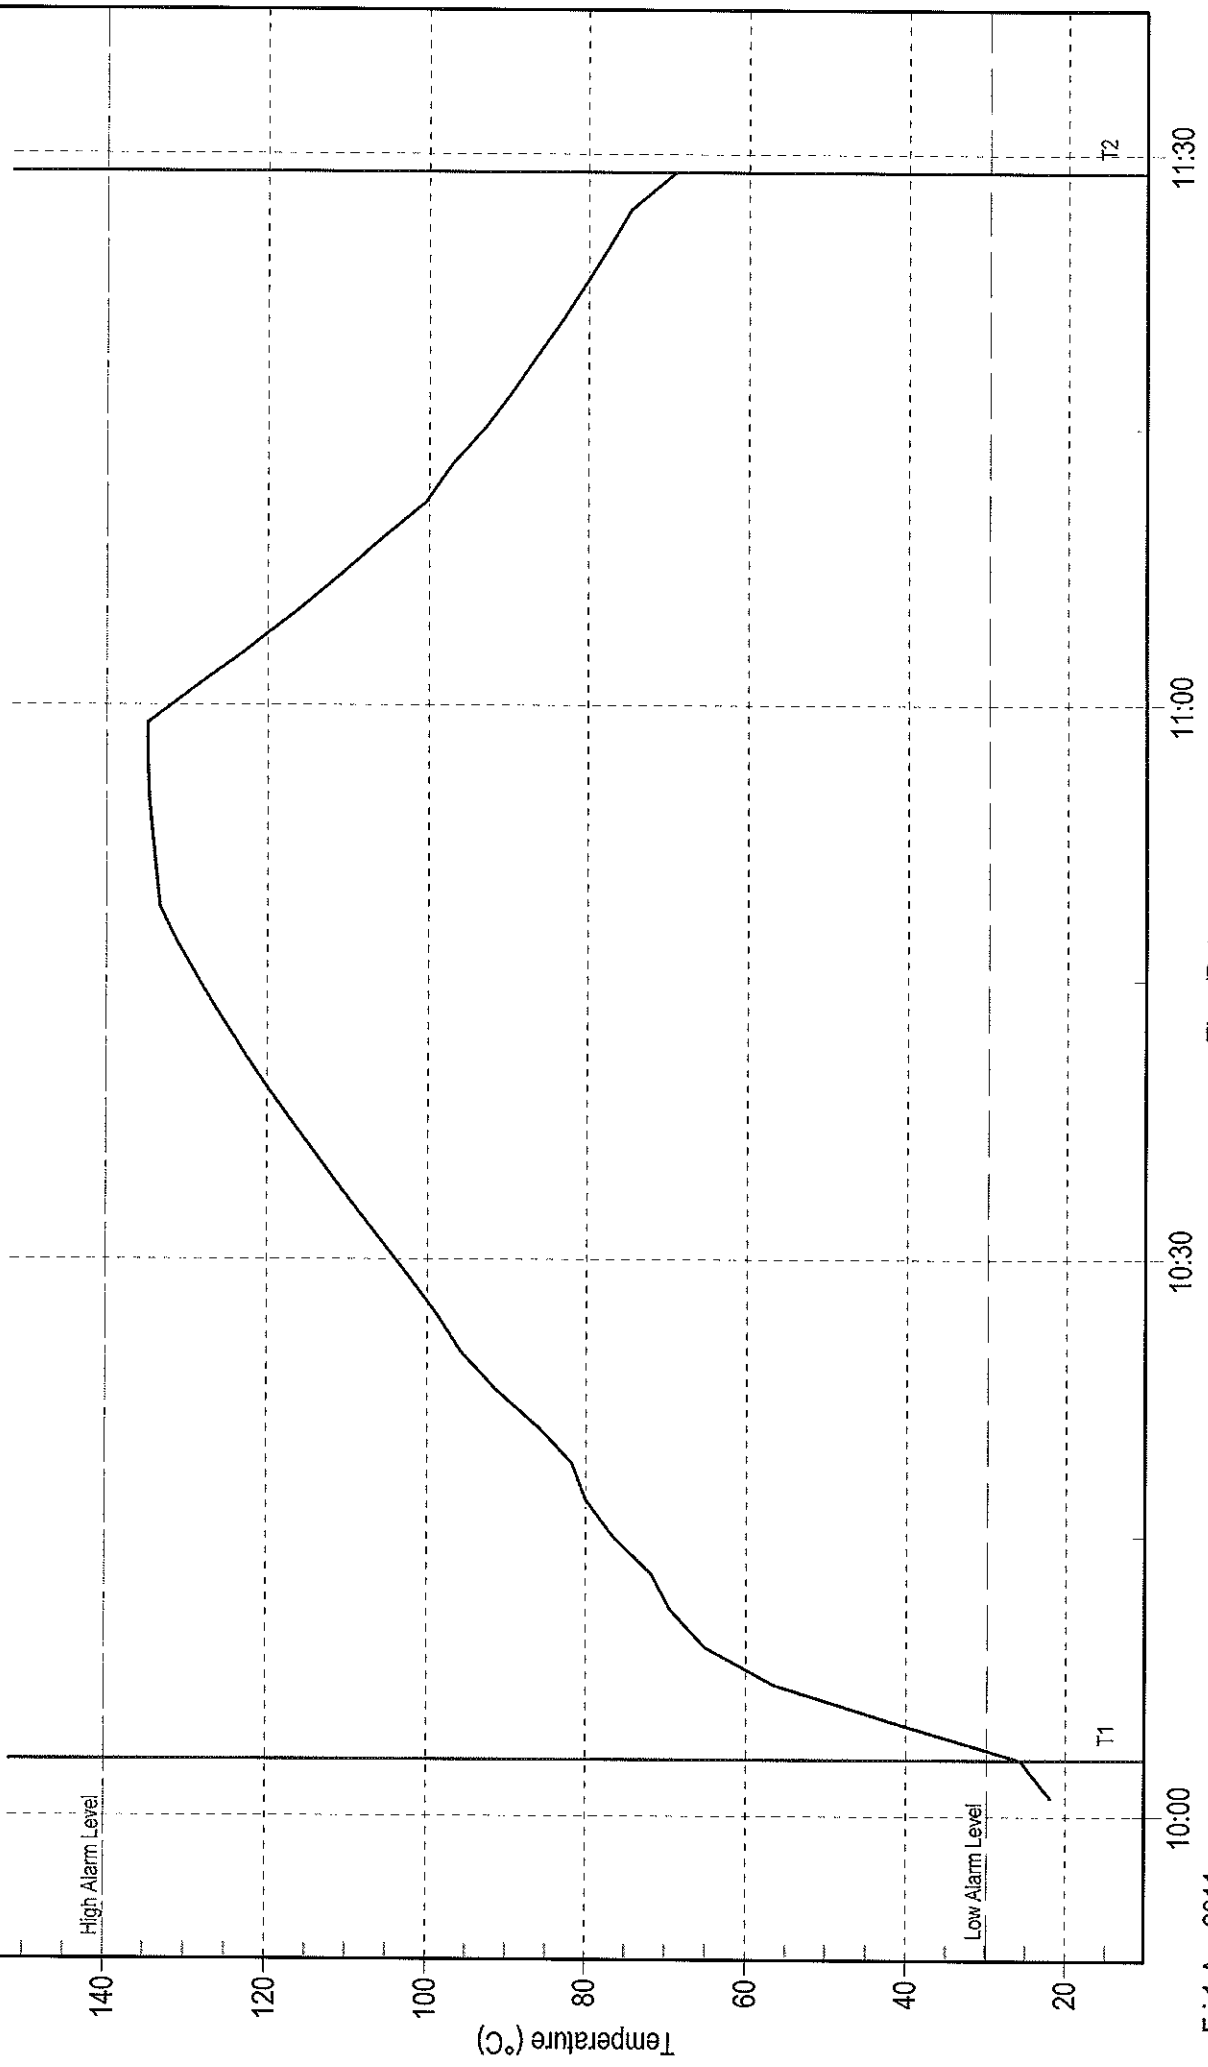

SL55T, Serial Number: 3400000015699F41

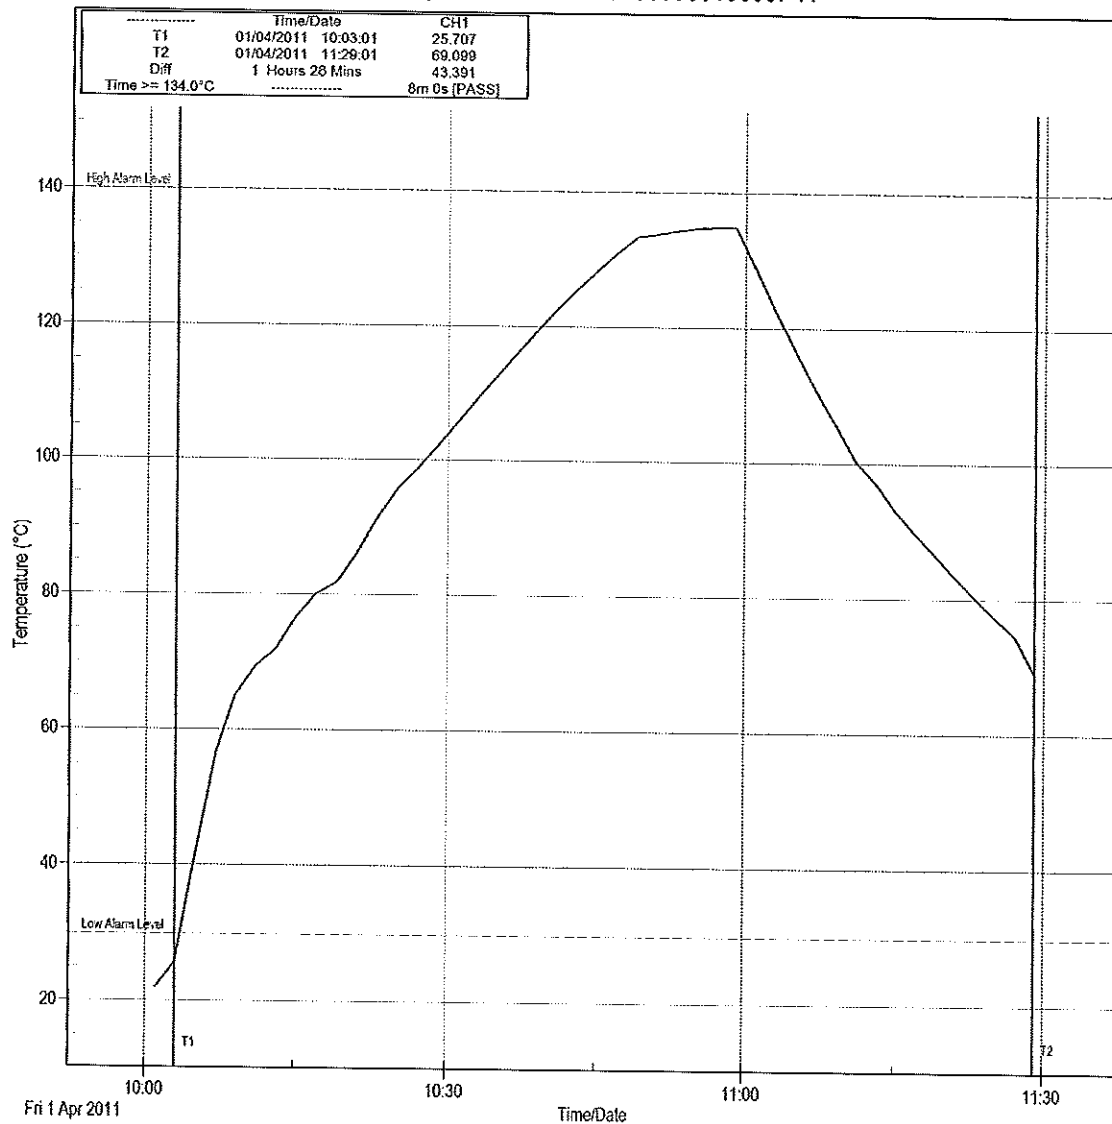

Type: SL55T

Readings: 45

User Manifest:

Log Interval (HH:MM:SS): 00:02:00

Serial Number: 3400000015699F41

Date of Calibration: 21 February 2011

| Channel | Description | Input Configuration | Max | Min | Mean | Deviation | MKT | Alarm |
|-----------|-------------|---------------------|-------|-------|-------|-----------|-------|-------|
| Channel 1 | CH1 | Temperature | 134.9 | 21.93 | 97.29 | 112.97 | 114.4 | True |

Signature 1:
 Print Name :
 Date :

Signature 2:
 Print Name :
 Date :

Cycle No. 000001_1

30/03/2011

Serial No. Z0278

Lab Media 121C : 15 3 Probes

C:\logsys\Z0278\data\000001_1.mbf

Test Person Kevin Taylor

Sign VALID ESIG

Date 30/03/2011 dd/mm/yyyy 14:19:41


Reviewed By:

Sign


Date dd/mm/yyyy

| Time | Tmp 1 °C | Tmp 2 °C | Tmp 3 °C |
|----------|---------------------|-------------|-------------|
| 00:00:00 | Cycle Started | | |
| 00:00:04 | 50.8 | 30.3 | 37.5 |
| 00:00:05 | 50.9 | 30.5 | 37.8 |
| 00:02:05 | 61.6 | 55.5 | 65.0 |
| 00:04:05 | 67.4 | 78.7 | 74.3 |
| 00:06:05 | 72.8 | 89.8 | 77.8 |
| 00:08:05 | 81.4 | 83.9 | 83.0 |
| 00:10:05 | 89.0 | 93.7 | 89.8 |
| 00:12:05 | 94.5 | 94.3 | 95.5 |
| 00:14:05 | 98.6 | 97.8 | 98.7 |
| 00:16:05 | 100.7 | 100.5 | 100.6 |
| 00:18:05 | 105.6 | 105.4 | 105.5 |
| 00:20:05 | 109.8 | 109.6 | 109.7 |
| 00:22:05 | 113.7 | 113.4 | 113.7 |
| 00:24:05 | 117.4 | 117.1 | 117.4 |
| 00:26:05 | 121.2 | 120.7 | 121.0 |
| 00:26:12 | 121.4 | 121.0 | 121.2 |
| 00:26:20 | 121.1 | 120.6 | 120.9 |
| 00:26:38 | 121.1 | 120.7 | 120.9 |
| 00:26:46 | Sterilisation Start | | |
| 00:26:46 | 121.4 | 121.0 | 121.3 |
| 00:28:05 | 122.0 | 121.6 | 121.9 |
| 00:30:05 | 122.8 | 122.4 | 122.7 |
| 00:32:05 | 122.9 | 122.5 | 122.7 |
| 00:34:05 | 122.7 | 122.3 | 122.6 |
| 00:36:05 | 123.0 | 122.6 | 122.9 |
| 00:38:05 | 123.2 | 122.8 | 123.1 |
| 00:40:05 | 123.1 | 122.7 | 122.9 |
| 00:42:05 | 122.9 | 122.5 | 122.8 |
| 00:43:43 | Sterilisation End | | |
| 00:43:46 | 121.1 | 120.7 | 120.9 |
| 00:44:05 | 120.0 | 119.5 | 119.8 |
| 00:46:05 | 113.2 | 112.8 | 113.1 |
| 00:48:05 | 107.3 | 107.0 | 107.2 |
| 00:50:05 | 100.8 | 100.8 | 100.9 |
| 00:52:05 | 92.4 | 97.2 | 97.6 |
| 00:54:05 | 85.7 | 93.2 | 93.5 |
| 00:56:05 | 81.8 | 88.9 | 89.5 |
| 00:58:05 | 77.8 | 85.0 | 85.9 |
| 01:00:05 | 74.7 | 81.2 | 82.5 |
| 01:02:05 | 71.4 | 77.7 | 79.5 |
| 01:03:33 | Cycle Complete | | |
| 01:03:33 | 69.7 | 76.4 | 78.3 |

Data Logger Test
 Cycle No. 000001_1
 Serial No. Z0278
LTE Scientific Limited
 C:\logsys\Z0278\data\000001_1.mbf
 30/03/2011
 Lab Media 121C : 15 3 Probes

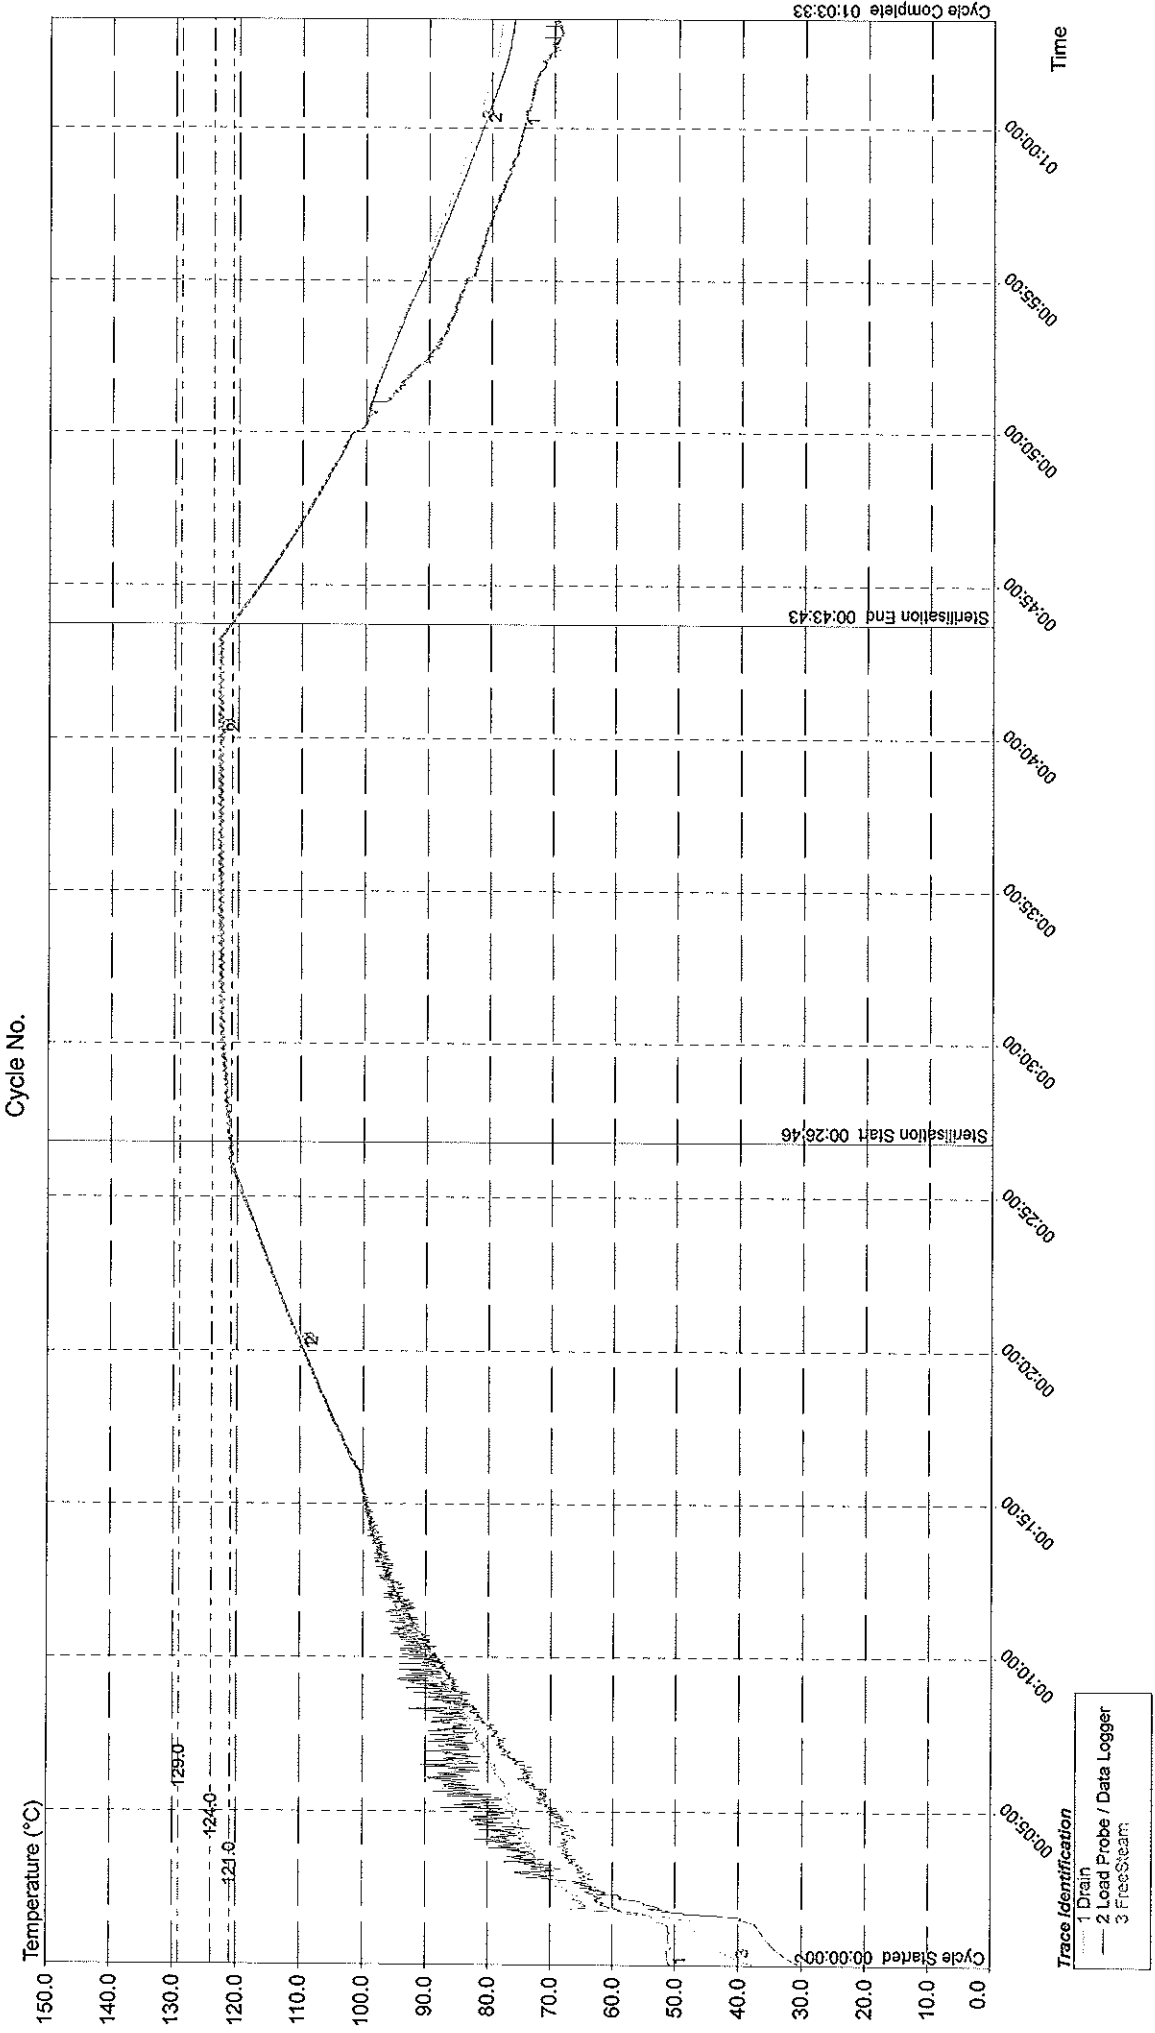


Data Logger Test
 Cycle No. 000001_1
 Serial No. Z0278
LTE Scientific Limited
 C:\logsys\Z0278\data\000001_1.mbf
 30/03/2011
 Lab Media 121C : 15 3 Probes

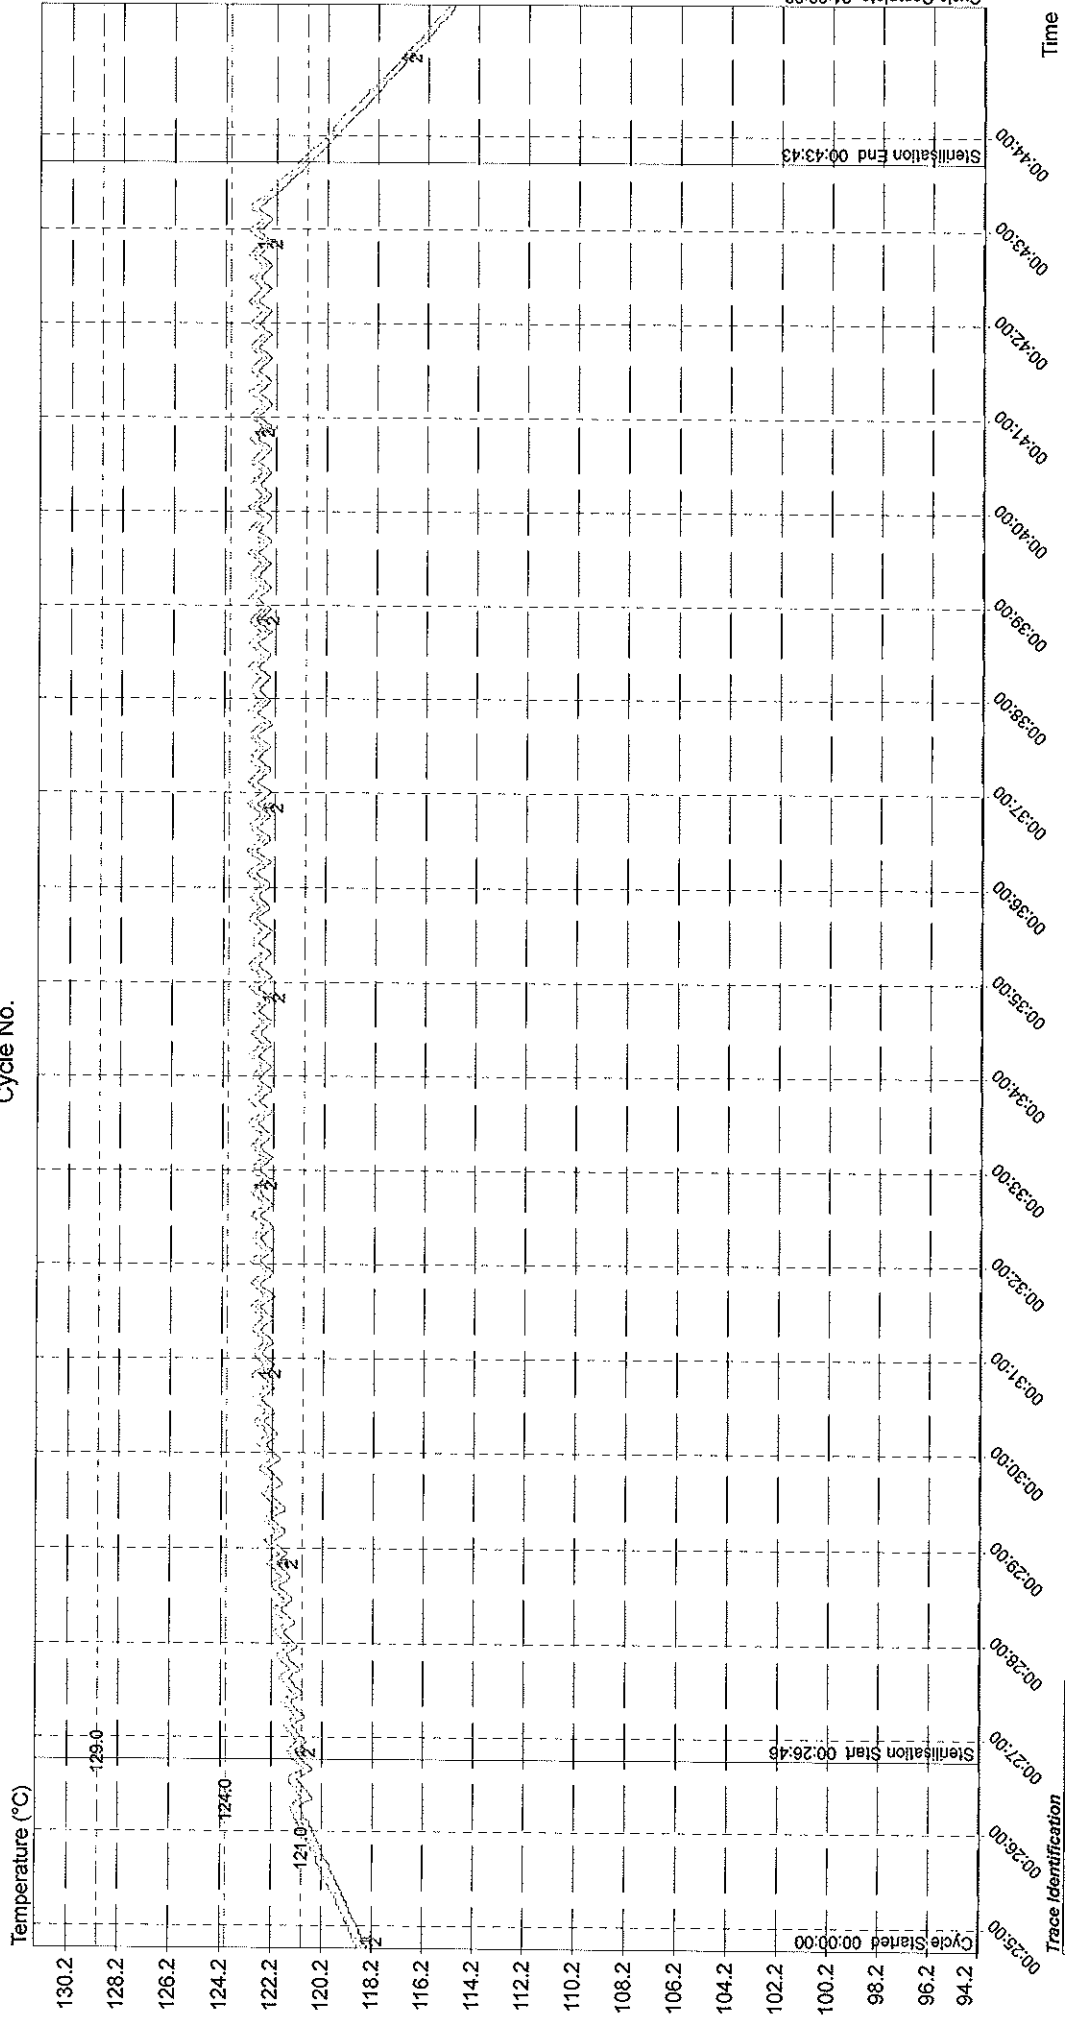

Trace Identification
 1 Drain
 2 Load Probe / Data Logger
 3 FreeSteam

SL55T, Serial Number: 3400000015699F41

| | |
|---------------------|--------------|
| Time/Date | CH1 |
| 29/03/2011 12:17:01 | 25.646 |
| 29/03/2011 13:25:01 | 63.404 |
| 1 Hours 8 Mins | 37.758 |
| Time >= 134.0°C | 0m 0s [FAIL] |

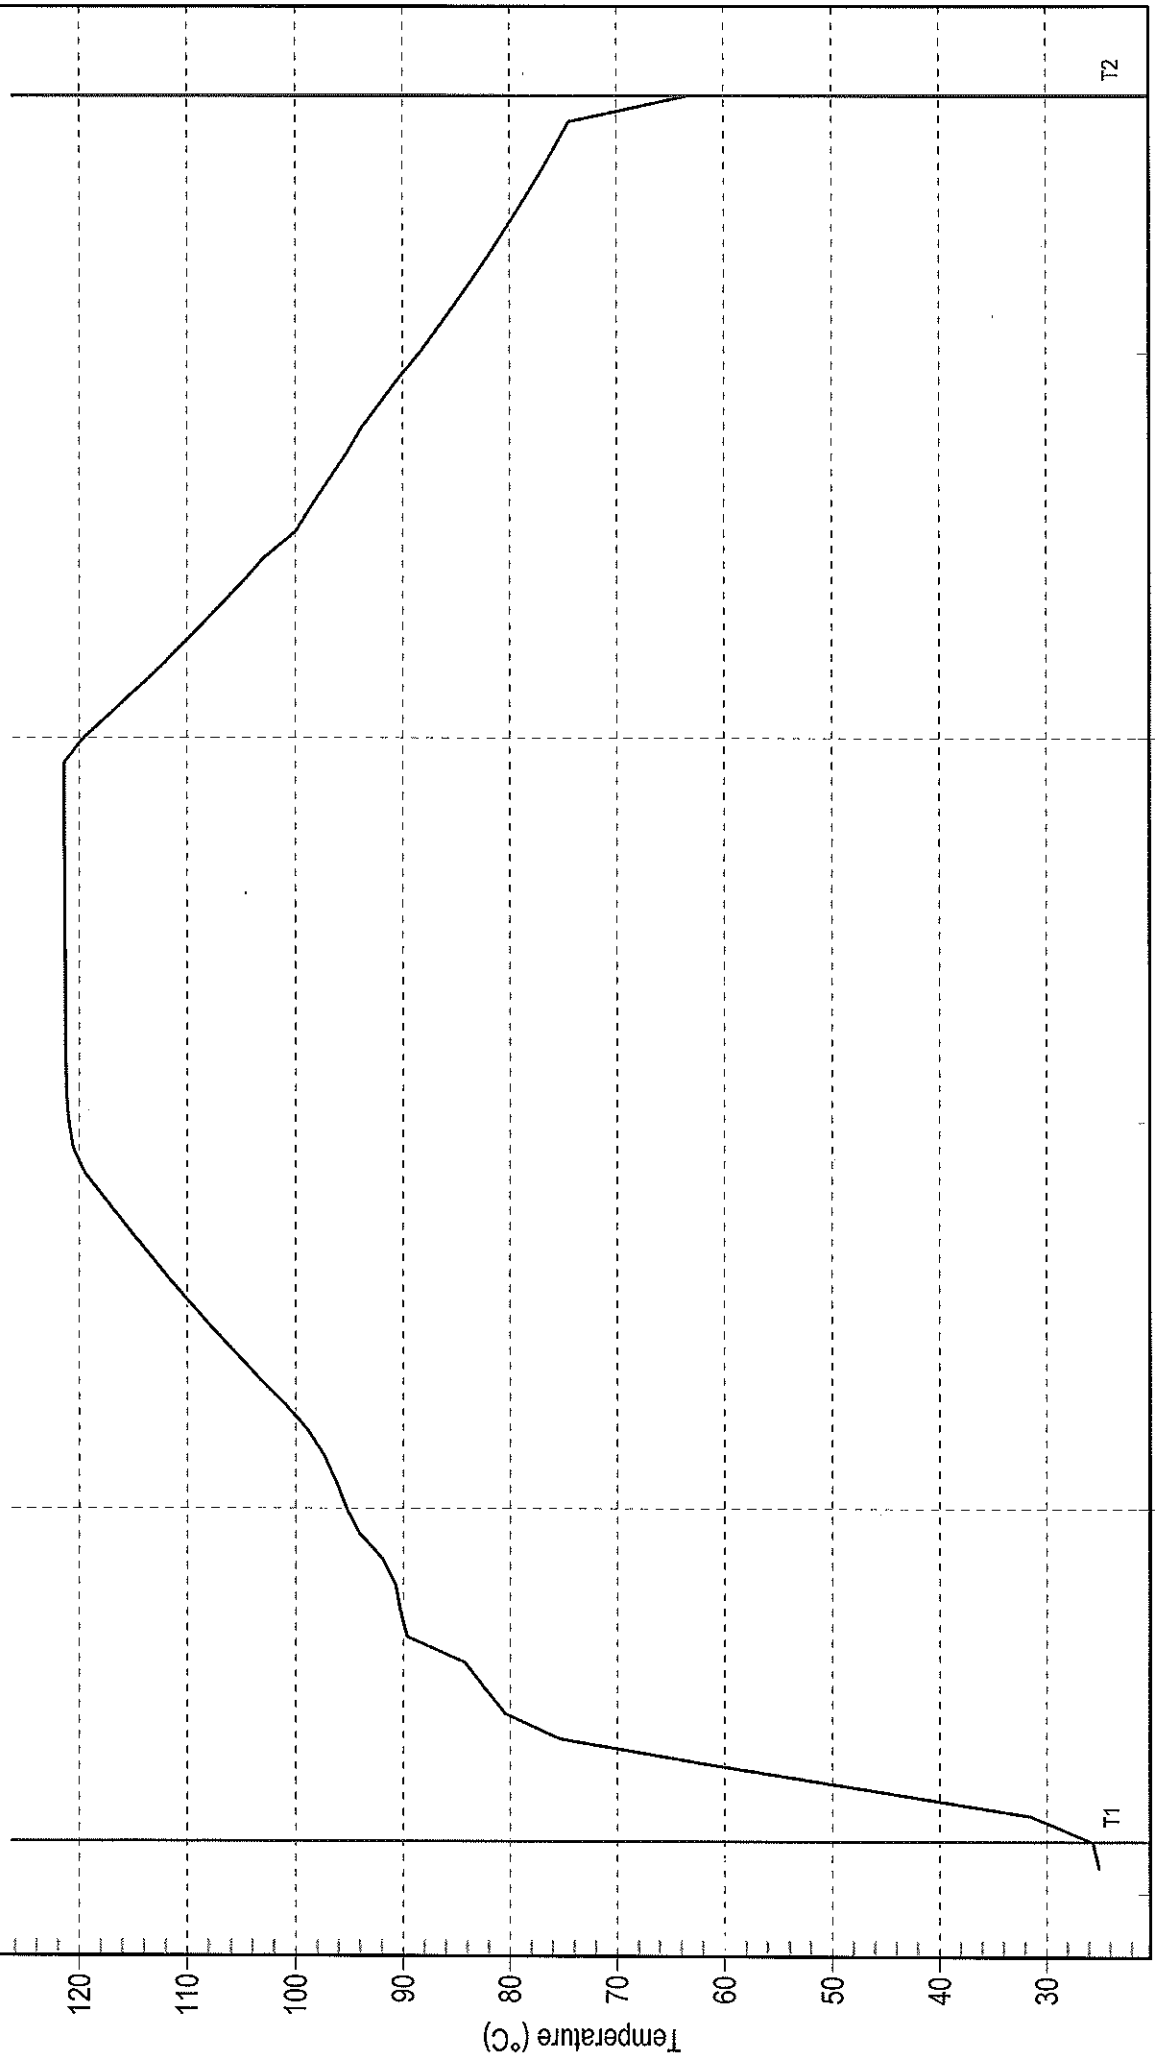

Tue 29 Mar 2011

12:30

13:00


Time/Date

Signature 1:
 Print Name:
 Date:

Signature 2:
 Print Name:
 Date:

| Channel | Description | Input Configuration | Max | Min | Mean | Deviation | MKT | Alarm |
|-----------|-------------|---------------------|--------|-------|--------|-----------|--------|-------|
| Channel 1 | CH1 | Temperature | 123.14 | 19.08 | 100.45 | 104.06 | 110.33 | True |

Type: SL55T
 Readings: 1983
 User Manifest:
 Log Interval (HH:MM:SS): 00:00:02
 Serial Number: 340000015699F41
 Date of Calibration: 21 February 2011

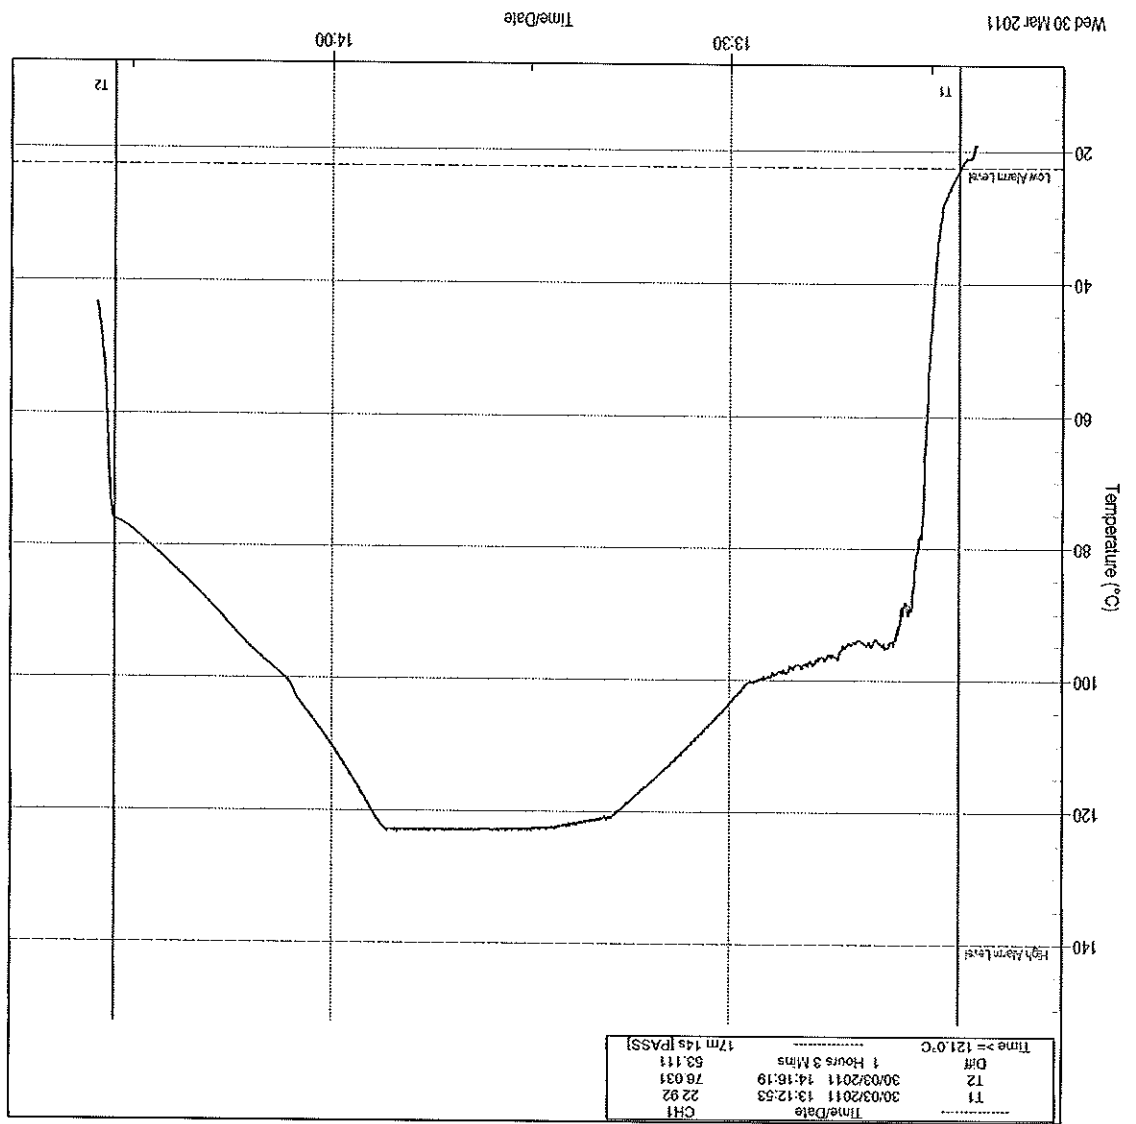

SL55T, Serial Number: 340000015699F41

SL55T, Serial Number: 3400000015699F41

| | Time/Date | CH1 |
|-----------------|---------------------|----------------|
| T1 | 30/03/2011 13:12:53 | 22.92 |
| T2 | 30/03/2011 14:16:19 | 76.031 |
| Diff | 1 Hours 3 Mins | 53.111 |
| Time >= 121.0°C | | 17m 14s [PASS] |



| | | |
|-----|------------------|--------|
| 838 | 30/03/2011 13:39 | 120.97 |
| 839 | 30/03/2011 13:39 | 121.12 |
| 840 | 30/03/2011 13:39 | 121.09 |
| 841 | 30/03/2011 13:39 | 121.21 |
| 842 | 30/03/2011 13:39 | 121.17 |
| 843 | 30/03/2011 13:39 | 120.91 |
| 844 | 30/03/2011 13:39 | 120.91 |
| 845 | 30/03/2011 13:39 | 120.91 |
| 846 | 30/03/2011 13:39 | 121.15 |
| 847 | 30/03/2011 13:39 | 121.17 |
| 848 | 30/03/2011 13:39 | 121.31 |
| 849 | 30/03/2011 13:39 | 121.27 |
| 850 | 30/03/2011 13:39 | 121.03 |
| 851 | 30/03/2011 13:39 | 121.03 |
| 852 | 30/03/2011 13:39 | 121.03 |
| 853 | 30/03/2011 13:39 | 121.03 |
| 854 | 30/03/2011 13:39 | 121.27 |
| 855 | 30/03/2011 13:40 | 121.29 |
| 856 | 30/03/2011 13:40 | 121.43 |
| 857 | 30/03/2011 13:40 | 121.4 |
| 858 | 30/03/2011 13:40 | 121.28 |
| 859 | 30/03/2011 13:40 | 121.22 |
| 860 | 30/03/2011 13:40 | 121.19 |
| 861 | 30/03/2011 13:40 | 121.18 |
| 862 | 30/03/2011 13:40 | 121.41 |
| 863 | 30/03/2011 13:40 | 121.42 |
| 864 | 30/03/2011 13:40 | 121.32 |
| 865 | 30/03/2011 13:40 | 121.27 |
| 866 | 30/03/2011 13:40 | 121.24 |
| 867 | 30/03/2011 13:40 | 121.23 |
| 868 | 30/03/2011 13:40 | 121.46 |
| 869 | 30/03/2011 13:40 | 121.47 |
| 870 | 30/03/2011 13:40 | 121.38 |
| 871 | 30/03/2011 13:40 | 121.57 |
| 872 | 30/03/2011 13:40 | 121.56 |
| 873 | 30/03/2011 13:40 | 121.45 |
| 874 | 30/03/2011 13:40 | 121.39 |
| 875 | 30/03/2011 13:40 | 121.36 |
| 876 | 30/03/2011 13:40 | 121.35 |
| 877 | 30/03/2011 13:40 | 121.58 |
| 878 | 30/03/2011 13:40 | 121.6 |
| 879 | 30/03/2011 13:40 | 121.4 |
| 880 | 30/03/2011 13:40 | 121.4 |
| 881 | 30/03/2011 13:40 | 121.4 |
| 882 | 30/03/2011 13:40 | 121.4 |
| 883 | 30/03/2011 13:40 | 121.64 |
| 884 | 30/03/2011 13:40 | 121.65 |
| 885 | 30/03/2011 13:41 | 121.56 |
| 886 | 30/03/2011 13:41 | 121.75 |
| 887 | 30/03/2011 13:41 | 121.74 |

| | | |
|-----|------------------|--------|
| 888 | 30/03/2011 13:41 | 121.63 |
| 889 | 30/03/2011 13:41 | 121.58 |
| 890 | 30/03/2011 13:41 | 121.56 |
| 891 | 30/03/2011 13:41 | 121.54 |
| 892 | 30/03/2011 13:41 | 121.77 |
| 893 | 30/03/2011 13:41 | 121.78 |
| 894 | 30/03/2011 13:41 | 121.68 |
| 895 | 30/03/2011 13:41 | 121.63 |
| 896 | 30/03/2011 13:41 | 121.61 |
| 897 | 30/03/2011 13:41 | 121.6 |
| 898 | 30/03/2011 13:41 | 121.83 |
| 899 | 30/03/2011 13:41 | 121.85 |
| 900 | 30/03/2011 13:41 | 121.99 |
| 901 | 30/03/2011 13:41 | 121.96 |
| 902 | 30/03/2011 13:41 | 121.71 |
| 903 | 30/03/2011 13:41 | 121.71 |
| 904 | 30/03/2011 13:41 | 121.71 |
| 905 | 30/03/2011 13:41 | 121.71 |
| 906 | 30/03/2011 13:41 | 121.95 |
| 907 | 30/03/2011 13:41 | 121.96 |
| 908 | 30/03/2011 13:41 | 121.78 |
| 909 | 30/03/2011 13:41 | 121.78 |
| 910 | 30/03/2011 13:41 | 121.78 |
| 911 | 30/03/2011 13:41 | 121.78 |
| 912 | 30/03/2011 13:41 | 122.01 |
| 913 | 30/03/2011 13:41 | 122.03 |
| 914 | 30/03/2011 13:41 | 122.18 |
| 915 | 30/03/2011 13:42 | 122.15 |
| 916 | 30/03/2011 13:42 | 121.84 |
| 917 | 30/03/2011 13:42 | 121.84 |
| 918 | 30/03/2011 13:42 | 121.84 |
| 919 | 30/03/2011 13:42 | 122.08 |
| 920 | 30/03/2011 13:42 | 122.1 |
| 921 | 30/03/2011 13:42 | 122.24 |
| 922 | 30/03/2011 13:42 | 122.21 |
| 923 | 30/03/2011 13:42 | 122.08 |
| 924 | 30/03/2011 13:42 | 122.02 |
| 925 | 30/03/2011 13:42 | 121.99 |
| 926 | 30/03/2011 13:42 | 121.97 |
| 927 | 30/03/2011 13:42 | 121.96 |
| 928 | 30/03/2011 13:42 | 122.19 |
| 929 | 30/03/2011 13:42 | 122.21 |
| 930 | 30/03/2011 13:42 | 122.11 |
| 931 | 30/03/2011 13:42 | 122.07 |
| 932 | 30/03/2011 13:42 | 122.04 |
| 933 | 30/03/2011 13:42 | 122.03 |
| 934 | 30/03/2011 13:42 | 122.26 |
| 935 | 30/03/2011 13:42 | 122.28 |
| 936 | 30/03/2011 13:42 | 122.18 |
| 937 | 30/03/2011 13:42 | 122.37 |

| | | |
|-----|------------------|--------|
| 938 | 30/03/2011 13:42 | 122.37 |
| 939 | 30/03/2011 13:42 | 122.15 |
| 940 | 30/03/2011 13:42 | 122.15 |
| 941 | 30/03/2011 13:42 | 122.15 |
| 942 | 30/03/2011 13:42 | 122.15 |
| 943 | 30/03/2011 13:42 | 122.39 |
| 944 | 30/03/2011 13:42 | 122.4 |
| 945 | 30/03/2011 13:43 | 122.31 |
| 946 | 30/03/2011 13:43 | 122.26 |
| 947 | 30/03/2011 13:43 | 122.24 |
| 948 | 30/03/2011 13:43 | 122.46 |
| 949 | 30/03/2011 13:43 | 122.47 |
| 950 | 30/03/2011 13:43 | 122.37 |
| 951 | 30/03/2011 13:43 | 122.56 |
| 952 | 30/03/2011 13:43 | 122.55 |
| 953 | 30/03/2011 13:43 | 122.44 |
| 954 | 30/03/2011 13:43 | 122.39 |
| 955 | 30/03/2011 13:43 | 122.36 |
| 956 | 30/03/2011 13:43 | 122.35 |
| 957 | 30/03/2011 13:43 | 122.34 |
| 958 | 30/03/2011 13:43 | 122.57 |
| 959 | 30/03/2011 13:43 | 122.58 |
| 960 | 30/03/2011 13:43 | 122.49 |
| 961 | 30/03/2011 13:43 | 122.44 |
| 962 | 30/03/2011 13:43 | 122.42 |
| 963 | 30/03/2011 13:43 | 122.41 |
| 964 | 30/03/2011 13:43 | 122.4 |
| 965 | 30/03/2011 13:43 | 122.4 |
| 966 | 30/03/2011 13:43 | 122.64 |
| 967 | 30/03/2011 13:43 | 122.65 |
| 968 | 30/03/2011 13:43 | 122.46 |
| 969 | 30/03/2011 13:43 | 122.46 |
| 970 | 30/03/2011 13:43 | 122.46 |
| 971 | 30/03/2011 13:43 | 122.46 |
| 972 | 30/03/2011 13:43 | 122.46 |
| 973 | 30/03/2011 13:43 | 122.46 |
| 974 | 30/03/2011 13:43 | 122.69 |
| 975 | 30/03/2011 13:44 | 122.46 |
| 976 | 30/03/2011 13:44 | 122.46 |
| 977 | 30/03/2011 13:44 | 122.46 |
| 978 | 30/03/2011 13:44 | 122.46 |
| 979 | 30/03/2011 13:44 | 122.46 |
| 980 | 30/03/2011 13:44 | 122.69 |
| 981 | 30/03/2011 13:44 | 122.71 |
| 982 | 30/03/2011 13:44 | 122.52 |
| 983 | 30/03/2011 13:44 | 122.52 |
| 984 | 30/03/2011 13:44 | 122.46 |
| 985 | 30/03/2011 13:44 | 122.46 |
| 986 | 30/03/2011 13:44 | 122.69 |
| 987 | 30/03/2011 13:44 | 122.71 |

| | | |
|------|------------------|--------|
| 988 | 30/03/2011 13:44 | 122.52 |
| 989 | 30/03/2011 13:44 | 122.52 |
| 990 | 30/03/2011 13:44 | 122.52 |
| 991 | 30/03/2011 13:44 | 122.52 |
| 992 | 30/03/2011 13:44 | 122.52 |
| 993 | 30/03/2011 13:44 | 122.52 |
| 994 | 30/03/2011 13:44 | 122.52 |
| 995 | 30/03/2011 13:44 | 122.75 |
| 996 | 30/03/2011 13:44 | 122.76 |
| 997 | 30/03/2011 13:44 | 122.58 |
| 998 | 30/03/2011 13:44 | 122.52 |
| 999 | 30/03/2011 13:44 | 122.52 |
| 1000 | 30/03/2011 13:44 | 122.52 |
| 1001 | 30/03/2011 13:44 | 122.75 |
| 1002 | 30/03/2011 13:44 | 122.76 |
| 1003 | 30/03/2011 13:44 | 122.91 |
| 1004 | 30/03/2011 13:44 | 122.58 |
| 1005 | 30/03/2011 13:45 | 122.58 |
| 1006 | 30/03/2011 13:45 | 122.58 |
| 1007 | 30/03/2011 13:45 | 122.58 |
| 1008 | 30/03/2011 13:45 | 122.58 |
| 1009 | 30/03/2011 13:45 | 122.58 |
| 1010 | 30/03/2011 13:45 | 122.82 |
| 1011 | 30/03/2011 13:45 | 122.83 |
| 1012 | 30/03/2011 13:45 | 122.58 |
| 1013 | 30/03/2011 13:45 | 122.58 |
| 1014 | 30/03/2011 13:45 | 122.58 |
| 1015 | 30/03/2011 13:45 | 122.58 |
| 1016 | 30/03/2011 13:45 | 122.82 |
| 1017 | 30/03/2011 13:45 | 122.83 |
| 1018 | 30/03/2011 13:45 | 122.74 |
| 1019 | 30/03/2011 13:45 | 122.69 |
| 1020 | 30/03/2011 13:45 | 122.58 |
| 1021 | 30/03/2011 13:45 | 122.58 |
| 1022 | 30/03/2011 13:45 | 122.58 |
| 1023 | 30/03/2011 13:45 | 122.82 |
| 1024 | 30/03/2011 13:45 | 122.83 |
| 1025 | 30/03/2011 13:45 | 122.74 |
| 1026 | 30/03/2011 13:45 | 122.69 |
| 1027 | 30/03/2011 13:45 | 122.67 |
| 1028 | 30/03/2011 13:45 | 122.58 |
| 1029 | 30/03/2011 13:45 | 122.58 |
| 1030 | 30/03/2011 13:45 | 122.82 |
| 1031 | 30/03/2011 13:45 | 122.83 |
| 1032 | 30/03/2011 13:45 | 122.74 |
| 1033 | 30/03/2011 13:45 | 122.69 |
| 1034 | 30/03/2011 13:45 | 122.67 |
| 1035 | 30/03/2011 13:46 | 122.65 |
| 1036 | 30/03/2011 13:46 | 122.65 |
| 1037 | 30/03/2011 13:46 | 122.65 |

| | | |
|------|------------------|--------|
| 1038 | 30/03/2011 13:46 | 122.65 |
| 1039 | 30/03/2011 13:46 | 122.65 |
| 1040 | 30/03/2011 13:46 | 122.65 |
| 1041 | 30/03/2011 13:46 | 122.65 |
| 1042 | 30/03/2011 13:46 | 122.65 |
| 1043 | 30/03/2011 13:46 | 122.65 |
| 1044 | 30/03/2011 13:46 | 122.65 |
| 1045 | 30/03/2011 13:46 | 122.65 |
| 1046 | 30/03/2011 13:46 | 122.65 |
| 1047 | 30/03/2011 13:46 | 122.89 |
| 1048 | 30/03/2011 13:46 | 122.64 |
| 1049 | 30/03/2011 13:46 | 122.64 |
| 1050 | 30/03/2011 13:46 | 122.64 |
| 1051 | 30/03/2011 13:46 | 122.64 |
| 1052 | 30/03/2011 13:46 | 122.64 |
| 1053 | 30/03/2011 13:46 | 122.64 |
| 1054 | 30/03/2011 13:46 | 122.88 |
| 1055 | 30/03/2011 13:46 | 122.64 |
| 1056 | 30/03/2011 13:46 | 122.64 |
| 1057 | 30/03/2011 13:46 | 122.64 |
| 1058 | 30/03/2011 13:46 | 122.64 |
| 1059 | 30/03/2011 13:46 | 122.64 |
| 1060 | 30/03/2011 13:46 | 122.88 |
| 1061 | 30/03/2011 13:46 | 122.9 |
| 1062 | 30/03/2011 13:46 | 122.81 |
| 1063 | 30/03/2011 13:46 | 122.64 |
| 1064 | 30/03/2011 13:46 | 122.64 |
| 1065 | 30/03/2011 13:47 | 122.64 |
| 1066 | 30/03/2011 13:47 | 122.64 |
| 1067 | 30/03/2011 13:47 | 122.64 |
| 1068 | 30/03/2011 13:47 | 122.88 |
| 1069 | 30/03/2011 13:47 | 122.9 |
| 1070 | 30/03/2011 13:47 | 122.81 |
| 1071 | 30/03/2011 13:47 | 122.64 |
| 1072 | 30/03/2011 13:47 | 122.64 |
| 1073 | 30/03/2011 13:47 | 122.64 |
| 1074 | 30/03/2011 13:47 | 122.64 |
| 1075 | 30/03/2011 13:47 | 122.88 |
| 1076 | 30/03/2011 13:47 | 122.9 |
| 1077 | 30/03/2011 13:47 | 122.81 |
| 1078 | 30/03/2011 13:47 | 122.64 |
| 1079 | 30/03/2011 13:47 | 122.64 |
| 1080 | 30/03/2011 13:47 | 122.64 |
| 1081 | 30/03/2011 13:47 | 122.64 |
| 1082 | 30/03/2011 13:47 | 122.88 |
| 1083 | 30/03/2011 13:47 | 122.9 |
| 1084 | 30/03/2011 13:47 | 122.81 |
| 1085 | 30/03/2011 13:47 | 122.76 |
| 1086 | 30/03/2011 13:47 | 122.64 |
| 1087 | 30/03/2011 13:47 | 122.64 |

| | | |
|------|------------------|--------|
| 1088 | 30/03/2011 13:47 | 122.64 |
| 1089 | 30/03/2011 13:47 | 122.88 |
| 1090 | 30/03/2011 13:47 | 122.9 |
| 1091 | 30/03/2011 13:47 | 122.81 |
| 1092 | 30/03/2011 13:47 | 122.76 |
| 1093 | 30/03/2011 13:47 | 122.74 |
| 1094 | 30/03/2011 13:47 | 122.64 |
| 1095 | 30/03/2011 13:48 | 122.78 |
| 1096 | 30/03/2011 13:48 | 122.85 |
| 1097 | 30/03/2011 13:48 | 122.78 |
| 1098 | 30/03/2011 13:48 | 122.74 |
| 1099 | 30/03/2011 13:48 | 122.72 |
| 1100 | 30/03/2011 13:48 | 122.71 |
| 1101 | 30/03/2011 13:48 | 122.71 |
| 1102 | 30/03/2011 13:48 | 122.71 |
| 1103 | 30/03/2011 13:48 | 122.71 |
| 1104 | 30/03/2011 13:48 | 122.71 |
| 1105 | 30/03/2011 13:48 | 122.71 |
| 1106 | 30/03/2011 13:48 | 122.71 |
| 1107 | 30/03/2011 13:48 | 122.71 |
| 1108 | 30/03/2011 13:48 | 122.71 |
| 1109 | 30/03/2011 13:48 | 122.71 |
| 1110 | 30/03/2011 13:48 | 122.71 |
| 1111 | 30/03/2011 13:48 | 122.71 |
| 1112 | 30/03/2011 13:48 | 122.71 |
| 1113 | 30/03/2011 13:48 | 122.71 |
| 1114 | 30/03/2011 13:48 | 122.71 |
| 1115 | 30/03/2011 13:48 | 122.71 |
| 1116 | 30/03/2011 13:48 | 122.71 |
| 1117 | 30/03/2011 13:48 | 122.71 |
| 1118 | 30/03/2011 13:48 | 122.71 |
| 1119 | 30/03/2011 13:48 | 122.94 |
| 1120 | 30/03/2011 13:48 | 122.71 |
| 1121 | 30/03/2011 13:48 | 122.71 |
| 1122 | 30/03/2011 13:48 | 122.71 |
| 1123 | 30/03/2011 13:48 | 122.71 |
| 1124 | 30/03/2011 13:48 | 122.71 |
| 1125 | 30/03/2011 13:49 | 122.94 |
| 1126 | 30/03/2011 13:49 | 122.96 |
| 1127 | 30/03/2011 13:49 | 122.86 |
| 1128 | 30/03/2011 13:49 | 122.82 |
| 1129 | 30/03/2011 13:49 | 122.71 |
| 1130 | 30/03/2011 13:49 | 122.71 |
| 1131 | 30/03/2011 13:49 | 122.71 |
| 1132 | 30/03/2011 13:49 | 122.94 |
| 1133 | 30/03/2011 13:49 | 122.96 |
| 1134 | 30/03/2011 13:49 | 122.86 |
| 1135 | 30/03/2011 13:49 | 122.82 |
| 1136 | 30/03/2011 13:49 | 122.79 |
| 1137 | 30/03/2011 13:49 | 122.71 |

| | | |
|------|------------------|--------|
| 1138 | 30/03/2011 13:49 | 122.71 |
| 1139 | 30/03/2011 13:49 | 122.71 |
| 1140 | 30/03/2011 13:49 | 122.94 |
| 1141 | 30/03/2011 13:49 | 122.96 |
| 1142 | 30/03/2011 13:49 | 122.86 |
| 1143 | 30/03/2011 13:49 | 122.82 |
| 1144 | 30/03/2011 13:49 | 122.71 |
| 1145 | 30/03/2011 13:49 | 122.71 |
| 1146 | 30/03/2011 13:49 | 122.94 |
| 1147 | 30/03/2011 13:49 | 122.96 |
| 1148 | 30/03/2011 13:49 | 122.86 |
| 1149 | 30/03/2011 13:49 | 122.82 |
| 1150 | 30/03/2011 13:49 | 122.79 |
| 1151 | 30/03/2011 13:49 | 122.71 |
| 1152 | 30/03/2011 13:49 | 122.71 |
| 1153 | 30/03/2011 13:49 | 122.94 |
| 1154 | 30/03/2011 13:49 | 122.96 |
| 1155 | 30/03/2011 13:50 | 122.86 |
| 1156 | 30/03/2011 13:50 | 122.82 |
| 1157 | 30/03/2011 13:50 | 122.79 |
| 1158 | 30/03/2011 13:50 | 122.78 |
| 1159 | 30/03/2011 13:50 | 122.71 |
| 1160 | 30/03/2011 13:50 | 122.71 |
| 1161 | 30/03/2011 13:50 | 122.94 |
| 1162 | 30/03/2011 13:50 | 122.96 |
| 1163 | 30/03/2011 13:50 | 122.86 |
| 1164 | 30/03/2011 13:50 | 122.82 |
| 1165 | 30/03/2011 13:50 | 122.79 |
| 1166 | 30/03/2011 13:50 | 122.71 |
| 1167 | 30/03/2011 13:50 | 122.71 |
| 1168 | 30/03/2011 13:50 | 122.94 |
| 1169 | 30/03/2011 13:50 | 122.96 |
| 1170 | 30/03/2011 13:50 | 122.86 |
| 1171 | 30/03/2011 13:50 | 122.82 |
| 1172 | 30/03/2011 13:50 | 122.79 |
| 1173 | 30/03/2011 13:50 | 122.71 |
| 1174 | 30/03/2011 13:50 | 122.71 |
| 1175 | 30/03/2011 13:50 | 122.94 |
| 1176 | 30/03/2011 13:50 | 122.96 |
| 1177 | 30/03/2011 13:50 | 122.86 |
| 1178 | 30/03/2011 13:50 | 122.82 |
| 1179 | 30/03/2011 13:50 | 122.79 |
| 1180 | 30/03/2011 13:50 | 122.78 |
| 1181 | 30/03/2011 13:50 | 122.71 |
| 1182 | 30/03/2011 13:50 | 122.71 |
| 1183 | 30/03/2011 13:50 | 122.94 |
| 1184 | 30/03/2011 13:50 | 122.96 |
| 1185 | 30/03/2011 13:51 | 122.86 |
| 1186 | 30/03/2011 13:51 | 122.82 |
| 1187 | 30/03/2011 13:51 | 122.79 |

| | | |
|------|------------------|--------|
| 1188 | 30/03/2011 13:51 | 122.71 |
| 1189 | 30/03/2011 13:51 | 122.71 |
| 1190 | 30/03/2011 13:51 | 122.94 |
| 1191 | 30/03/2011 13:51 | 122.96 |
| 1192 | 30/03/2011 13:51 | 122.86 |
| 1193 | 30/03/2011 13:51 | 122.82 |
| 1194 | 30/03/2011 13:51 | 122.79 |
| 1195 | 30/03/2011 13:51 | 122.78 |
| 1196 | 30/03/2011 13:51 | 122.71 |
| 1197 | 30/03/2011 13:51 | 122.84 |
| 1198 | 30/03/2011 13:51 | 122.9 |
| 1199 | 30/03/2011 13:51 | 122.83 |
| 1200 | 30/03/2011 13:51 | 123.04 |
| 1201 | 30/03/2011 13:51 | 122.77 |
| 1202 | 30/03/2011 13:51 | 122.77 |
| 1203 | 30/03/2011 13:51 | 122.71 |
| 1204 | 30/03/2011 13:51 | 122.84 |
| 1205 | 30/03/2011 13:51 | 122.9 |
| 1206 | 30/03/2011 13:51 | 122.83 |
| 1207 | 30/03/2011 13:51 | 122.8 |
| 1208 | 30/03/2011 13:51 | 122.79 |
| 1209 | 30/03/2011 13:51 | 122.78 |
| 1210 | 30/03/2011 13:51 | 122.77 |
| 1211 | 30/03/2011 13:51 | 122.77 |
| 1212 | 30/03/2011 13:51 | 122.77 |
| 1213 | 30/03/2011 13:51 | 122.77 |
| 1214 | 30/03/2011 13:51 | 122.77 |
| 1215 | 30/03/2011 13:52 | 122.77 |
| 1216 | 30/03/2011 13:52 | 122.77 |
| 1217 | 30/03/2011 13:52 | 122.77 |
| 1218 | 30/03/2011 13:52 | 122.77 |
| 1219 | 30/03/2011 13:52 | 122.77 |
| 1220 | 30/03/2011 13:52 | 122.77 |
| 1221 | 30/03/2011 13:52 | 123 |
| 1222 | 30/03/2011 13:52 | 122.77 |
| 1223 | 30/03/2011 13:52 | 122.77 |
| 1224 | 30/03/2011 13:52 | 122.77 |
| 1225 | 30/03/2011 13:52 | 122.77 |
| 1226 | 30/03/2011 13:52 | 122.77 |
| 1227 | 30/03/2011 13:52 | 122.77 |
| 1228 | 30/03/2011 13:52 | 122.77 |
| 1229 | 30/03/2011 13:52 | 122.77 |
| 1230 | 30/03/2011 13:52 | 122.77 |
| 1231 | 30/03/2011 13:52 | 122.77 |
| 1232 | 30/03/2011 13:52 | 122.71 |
| 1233 | 30/03/2011 13:52 | 122.84 |
| 1234 | 30/03/2011 13:52 | 122.9 |
| 1235 | 30/03/2011 13:52 | 122.83 |
| 1236 | 30/03/2011 13:52 | 123.04 |
| 1237 | 30/03/2011 13:52 | 122.77 |

| | | |
|------|------------------|--------|
| 1238 | 30/03/2011 13:52 | 122.77 |
| 1239 | 30/03/2011 13:52 | 122.77 |
| 1240 | 30/03/2011 13:52 | 122.71 |
| 1241 | 30/03/2011 13:52 | 122.84 |
| 1242 | 30/03/2011 13:52 | 122.9 |
| 1243 | 30/03/2011 13:52 | 122.83 |
| 1244 | 30/03/2011 13:52 | 122.8 |
| 1245 | 30/03/2011 13:53 | 122.79 |
| 1246 | 30/03/2011 13:53 | 122.71 |
| 1247 | 30/03/2011 13:53 | 122.71 |
| 1248 | 30/03/2011 13:53 | 122.94 |
| 1249 | 30/03/2011 13:53 | 122.96 |
| 1250 | 30/03/2011 13:53 | 122.86 |
| 1251 | 30/03/2011 13:53 | 122.82 |
| 1252 | 30/03/2011 13:53 | 122.79 |
| 1253 | 30/03/2011 13:53 | 122.78 |
| 1254 | 30/03/2011 13:53 | 122.71 |
| 1255 | 30/03/2011 13:53 | 122.84 |
| 1256 | 30/03/2011 13:53 | 122.9 |
| 1257 | 30/03/2011 13:53 | 122.83 |
| 1258 | 30/03/2011 13:53 | 122.8 |
| 1259 | 30/03/2011 13:53 | 122.79 |
| 1260 | 30/03/2011 13:53 | 122.78 |
| 1261 | 30/03/2011 13:53 | 122.71 |
| 1262 | 30/03/2011 13:53 | 122.71 |
| 1263 | 30/03/2011 13:53 | 122.94 |
| 1264 | 30/03/2011 13:53 | 122.96 |
| 1265 | 30/03/2011 13:53 | 122.86 |
| 1266 | 30/03/2011 13:53 | 122.82 |
| 1267 | 30/03/2011 13:53 | 122.79 |
| 1268 | 30/03/2011 13:53 | 122.71 |
| 1269 | 30/03/2011 13:53 | 122.71 |
| 1270 | 30/03/2011 13:53 | 122.94 |
| 1271 | 30/03/2011 13:53 | 122.96 |
| 1272 | 30/03/2011 13:53 | 122.86 |
| 1273 | 30/03/2011 13:53 | 122.82 |
| 1274 | 30/03/2011 13:53 | 122.79 |
| 1275 | 30/03/2011 13:54 | 122.71 |
| 1276 | 30/03/2011 13:54 | 122.71 |
| 1277 | 30/03/2011 13:54 | 122.71 |
| 1278 | 30/03/2011 13:54 | 122.94 |
| 1279 | 30/03/2011 13:54 | 122.96 |
| 1280 | 30/03/2011 13:54 | 122.86 |
| 1281 | 30/03/2011 13:54 | 122.82 |
| 1282 | 30/03/2011 13:54 | 122.79 |
| 1283 | 30/03/2011 13:54 | 122.71 |
| 1284 | 30/03/2011 13:54 | 122.71 |
| 1285 | 30/03/2011 13:54 | 122.94 |
| 1286 | 30/03/2011 13:54 | 122.96 |
| 1287 | 30/03/2011 13:54 | 122.86 |

| | | |
|------|------------------|--------|
| 1288 | 30/03/2011 13:54 | 122.82 |
| 1289 | 30/03/2011 13:54 | 122.79 |
| 1290 | 30/03/2011 13:54 | 122.71 |
| 1291 | 30/03/2011 13:54 | 122.84 |
| 1292 | 30/03/2011 13:54 | 122.9 |
| 1293 | 30/03/2011 13:54 | 122.83 |
| 1294 | 30/03/2011 13:54 | 122.8 |
| 1295 | 30/03/2011 13:54 | 122.79 |
| 1296 | 30/03/2011 13:54 | 122.78 |
| 1297 | 30/03/2011 13:54 | 122.77 |
| 1298 | 30/03/2011 13:54 | 122.77 |
| 1299 | 30/03/2011 13:54 | 122.71 |
| 1300 | 30/03/2011 13:54 | 122.84 |
| 1301 | 30/03/2011 13:54 | 122.9 |
| 1302 | 30/03/2011 13:54 | 122.83 |
| 1303 | 30/03/2011 13:54 | 122.8 |
| 1304 | 30/03/2011 13:54 | 122.79 |
| 1305 | 30/03/2011 13:55 | 122.78 |
| 1306 | 30/03/2011 13:55 | 122.71 |
| 1307 | 30/03/2011 13:55 | 122.84 |
| 1308 | 30/03/2011 13:55 | 123.14 |
| 1309 | 30/03/2011 13:55 | 122.77 |
| 1310 | 30/03/2011 13:55 | 122.77 |
| 1311 | 30/03/2011 13:55 | 122.77 |
| 1312 | 30/03/2011 13:55 | 122.77 |
| 1313 | 30/03/2011 13:55 | 122.71 |
| 1314 | 30/03/2011 13:55 | 122.84 |
| 1315 | 30/03/2011 13:55 | 122.9 |
| 1316 | 30/03/2011 13:55 | 122.83 |
| 1317 | 30/03/2011 13:55 | 122.8 |
| 1318 | 30/03/2011 13:55 | 122.79 |
| 1319 | 30/03/2011 13:55 | 122.78 |
| 1320 | 30/03/2011 13:55 | 122.77 |
| 1321 | 30/03/2011 13:55 | 122.77 |
| 1322 | 30/03/2011 13:55 | 122.77 |
| 1323 | 30/03/2011 13:55 | 122.77 |
| 1324 | 30/03/2011 13:55 | 122.77 |
| 1325 | 30/03/2011 13:55 | 122.77 |
| 1326 | 30/03/2011 13:55 | 122.77 |
| 1327 | 30/03/2011 13:55 | 122.77 |
| 1328 | 30/03/2011 13:55 | 122.77 |
| 1329 | 30/03/2011 13:55 | 122.77 |
| 1330 | 30/03/2011 13:55 | 122.77 |
| 1331 | 30/03/2011 13:55 | 122.77 |
| 1332 | 30/03/2011 13:55 | 123 |
| 1333 | 30/03/2011 13:55 | 122.77 |
| 1334 | 30/03/2011 13:55 | 122.77 |
| 1335 | 30/03/2011 13:56 | 122.71 |
| 1336 | 30/03/2011 13:56 | 122.71 |
| 1337 | 30/03/2011 13:56 | 122.64 |

| | | |
|------|------------------|--------|
| 1338 | 30/03/2011 13:56 | 122.58 |
| 1339 | 30/03/2011 13:56 | 122.52 |
| 1340 | 30/03/2011 13:56 | 122.4 |
| 1341 | 30/03/2011 13:56 | 122.33 |
| 1342 | 30/03/2011 13:56 | 122.27 |
| 1343 | 30/03/2011 13:56 | 122.15 |
| 1344 | 30/03/2011 13:56 | 122.09 |
| 1345 | 30/03/2011 13:56 | 122.02 |
| 1346 | 30/03/2011 13:56 | 121.9 |
| 1347 | 30/03/2011 13:56 | 121.84 |
| 1348 | 30/03/2011 13:56 | 121.71 |
| 1349 | 30/03/2011 13:56 | 121.65 |
| 1350 | 30/03/2011 13:56 | 121.53 |
| 1351 | 30/03/2011 13:56 | 121.4 |
| 1352 | 30/03/2011 13:56 | 121.34 |
| 1353 | 30/03/2011 13:56 | 121.22 |
| 1354 | 30/03/2011 13:56 | 121.16 |
| 1355 | 30/03/2011 13:56 | 121.03 |
| 1356 | 30/03/2011 13:56 | 120.91 |